


SPD ECAL

Status Report 2023



**Oleg Gavrihuk, Laboratory of High Energy Physics, Dubna,
Russia**

- 1. ECAL position inside of Cryostat**
- 2. ECAL New Sizes corrected in 2023**
- 3. Test results with new SiPm EQR15 11-6060D-S**
 - 1. New Sipm testing results**
 - 2. EC prototype cells 40x40 Cosmic test**
- 4. Matrix form for new scintillator production (40x40x1.5 mm³)**
- 5. End Cup part of 256 cells plan to produce during of 2024**


ECAL with New Sizes in 2023

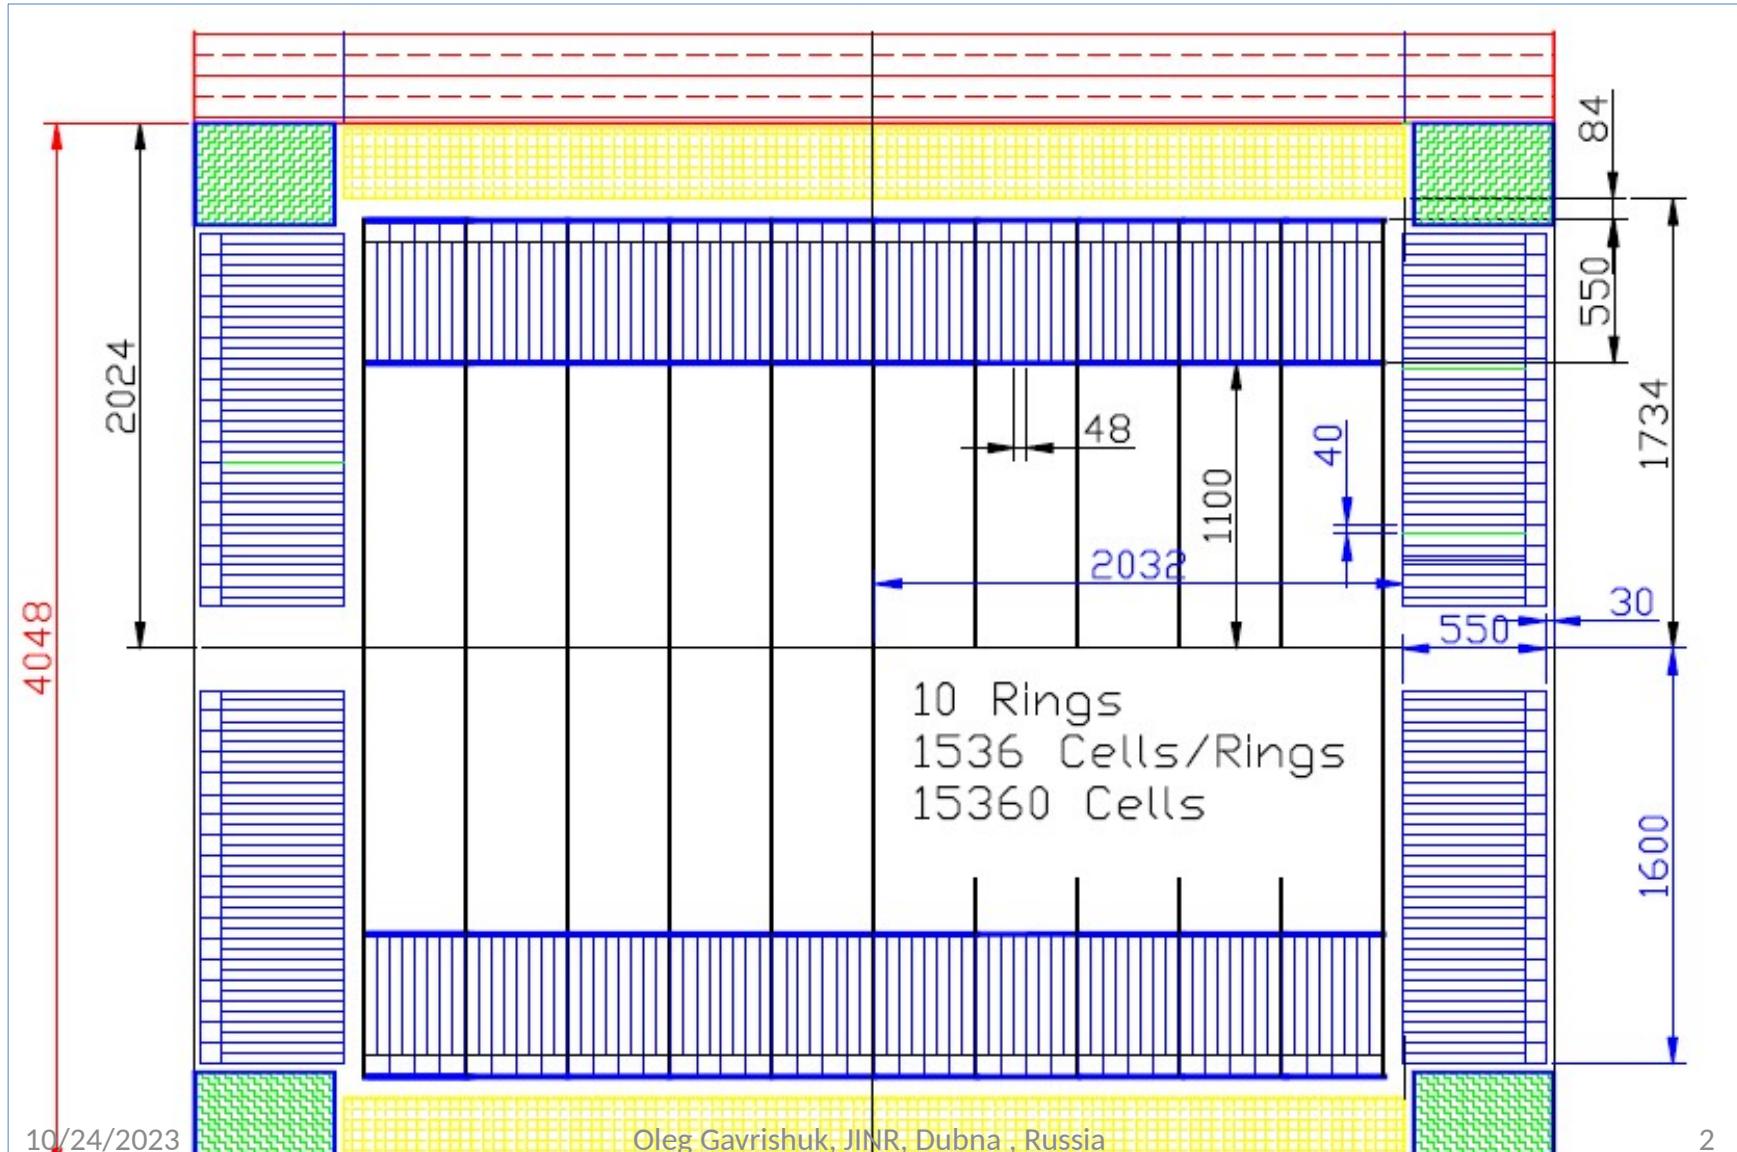

ECAL with New Sizes in 2023

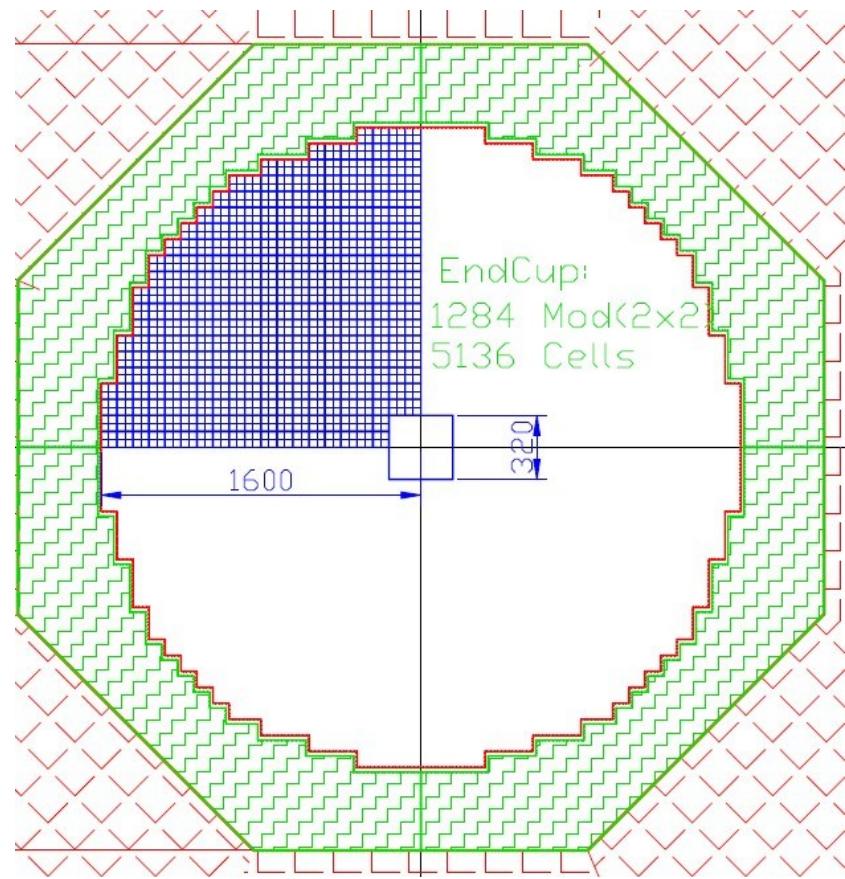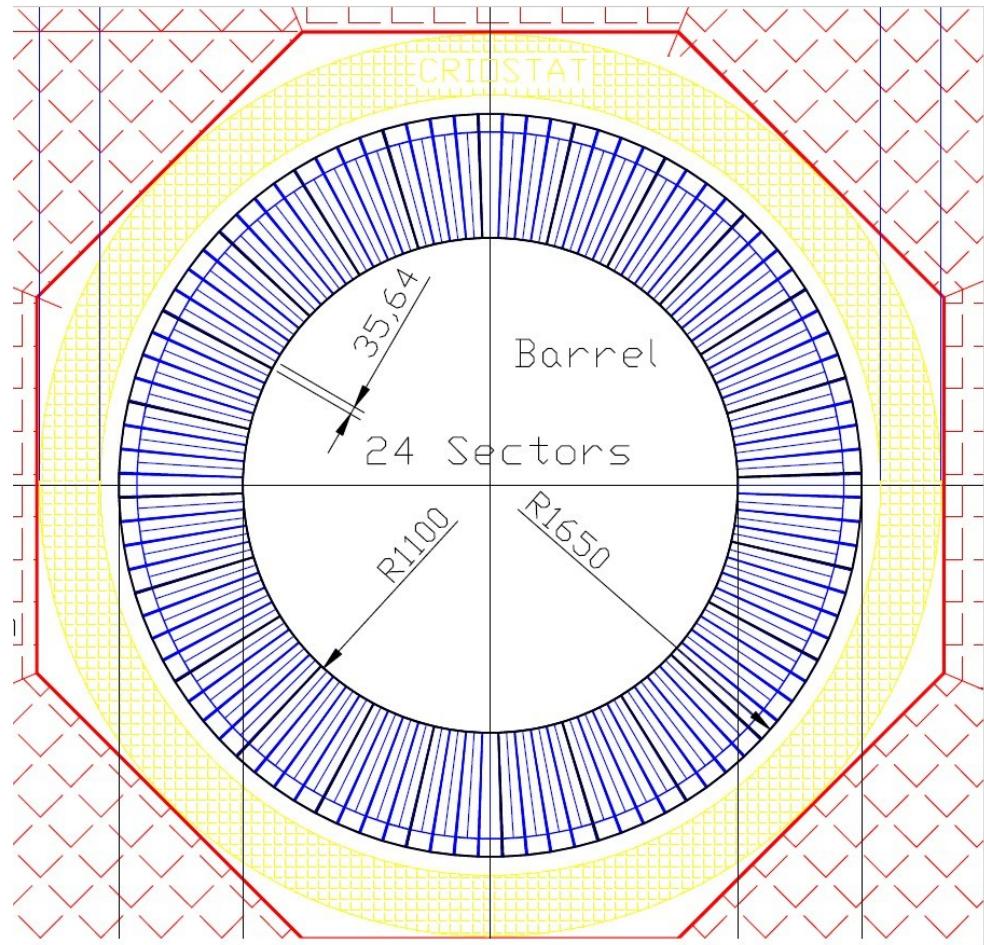

ECAL composition with New Sizes in 2023

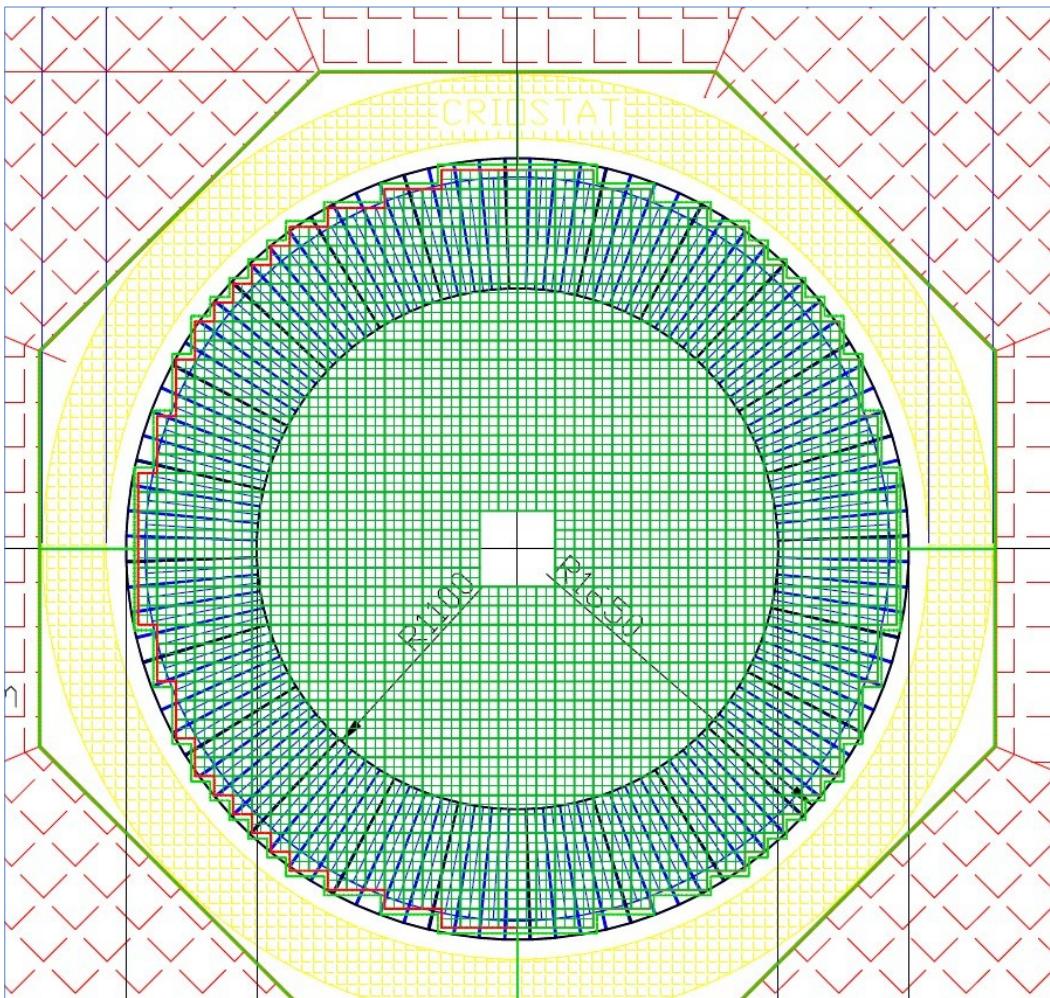



Barrel :

1. 10 Rings – 1536 cells/Ring
2. Total Cells – 15360
3. ADC64 – 240
4. 16ch Amplifiers – 960
5. Power units – 24
6. Weight – 38.4 tonn


2 END CUP:

1. Cells – 5136 / per End Cup
2. Total cells – 10272
3. ADC64 – 160
4. 16ch Amplifiers – 642
5. Power units – 20
6. Total Weight – 25.6 ton


ECAL 3D View Barrel and Cup parts

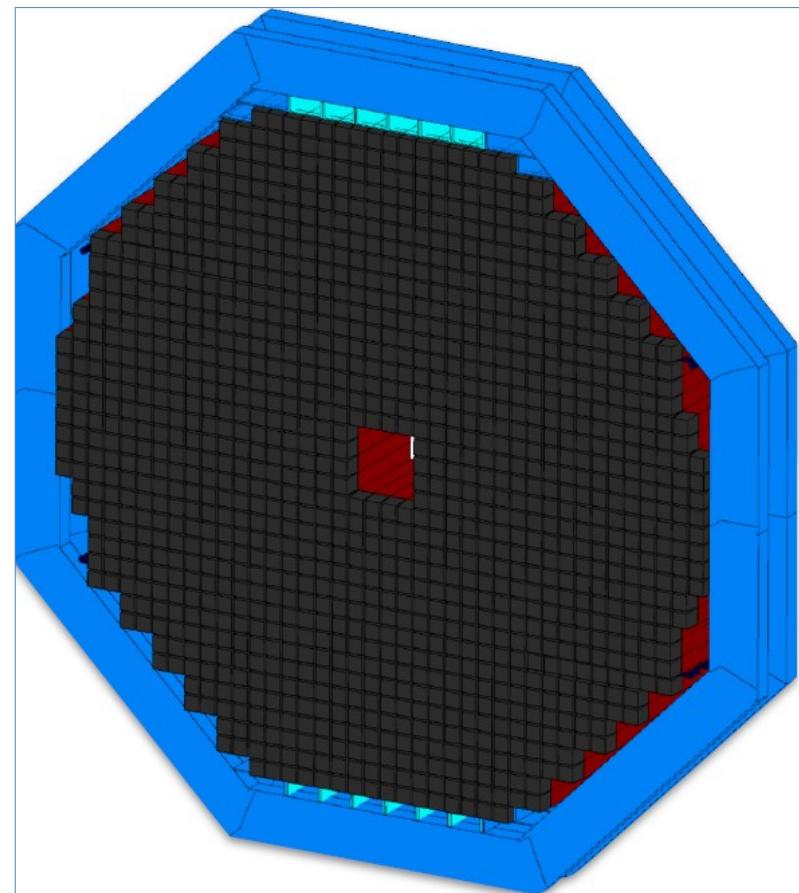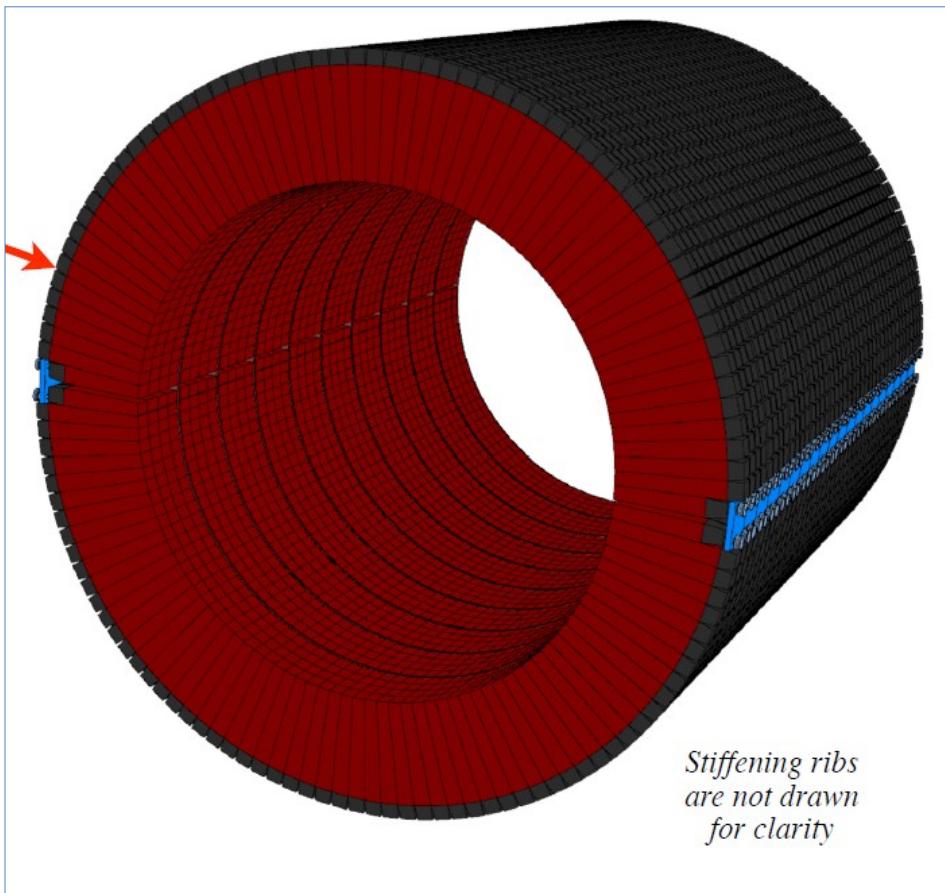

ECAL integration inside of SPD

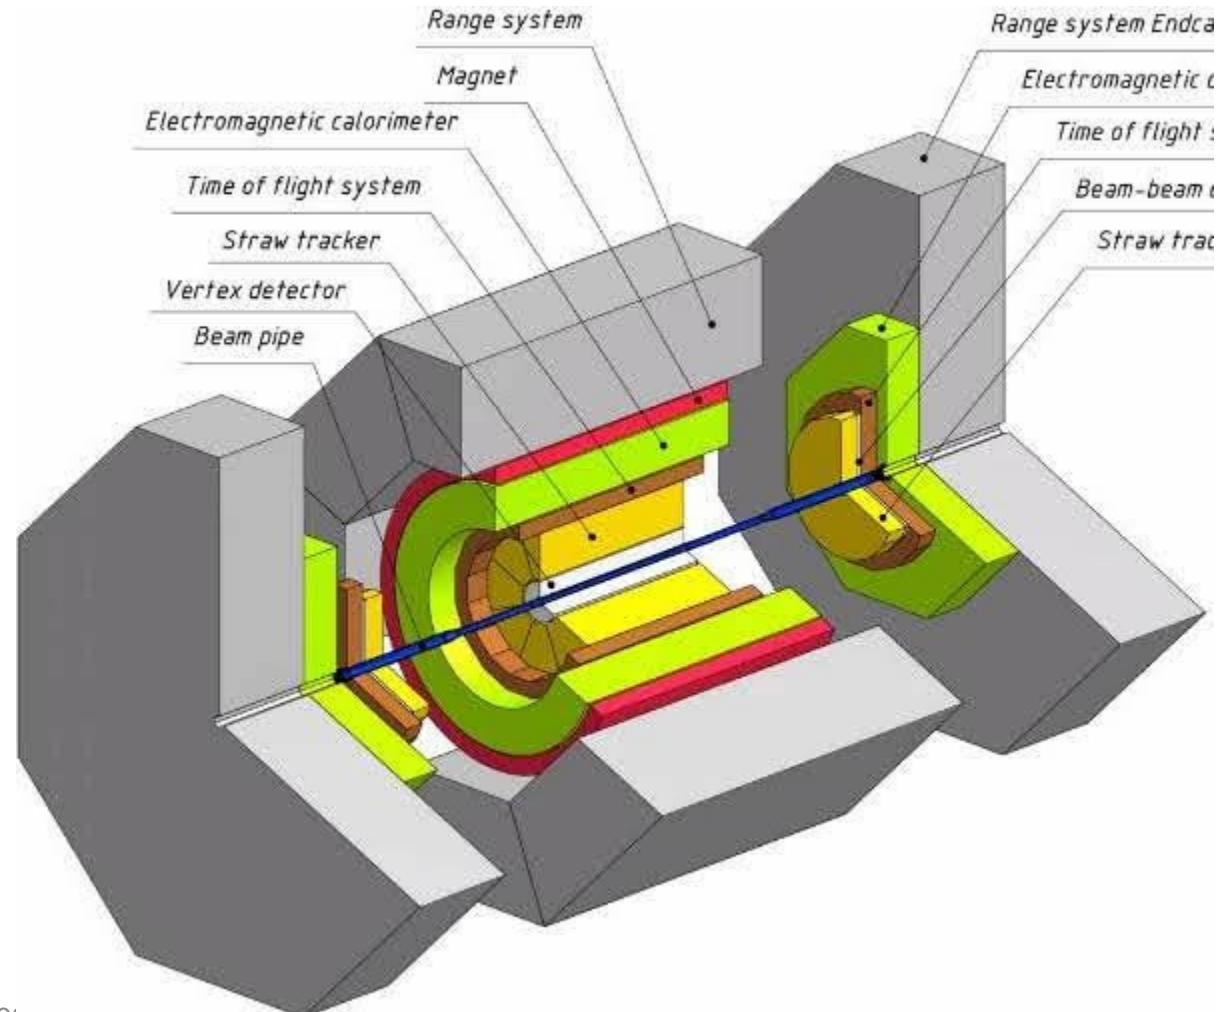

Test results with cosmic particles

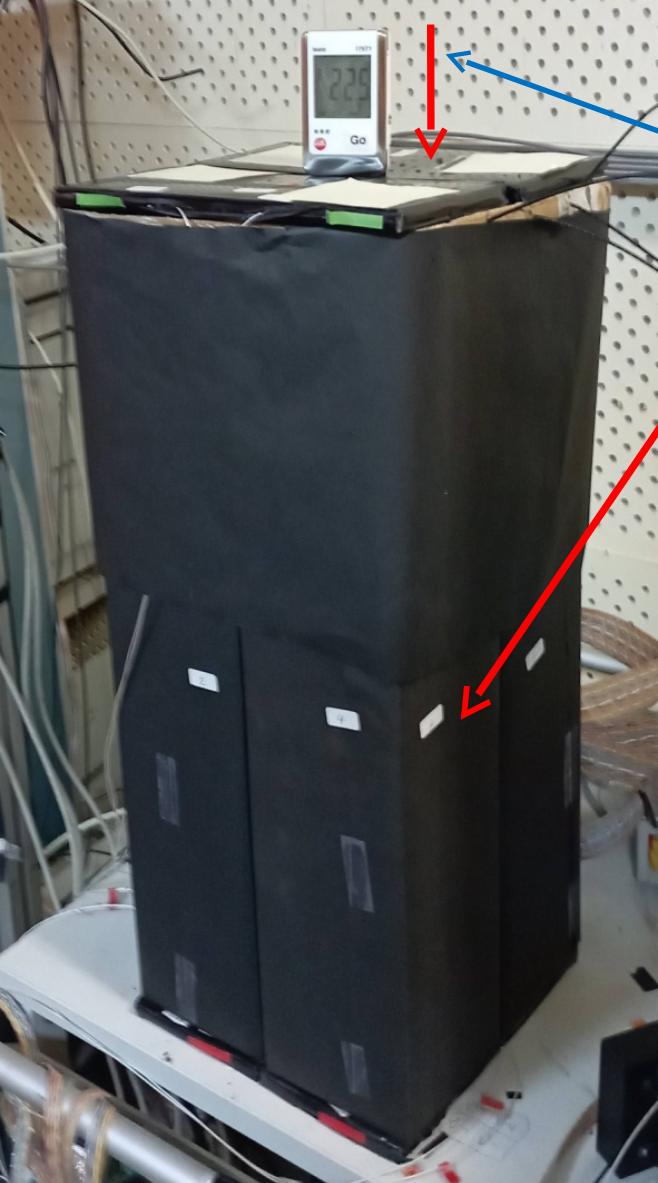

Cosmic Rays


Setup of 4 modules.
Each module consist from 9 cells of 4x4 cm². Totally tested 36 cells.

Sampling:


- 1.5 mm Scintillator
- 0.3 mm Lead
- 200 layers

Scintillator composition:

- Polyesterene
- 1.5% Paterphenyle
- 0.04% POPOP

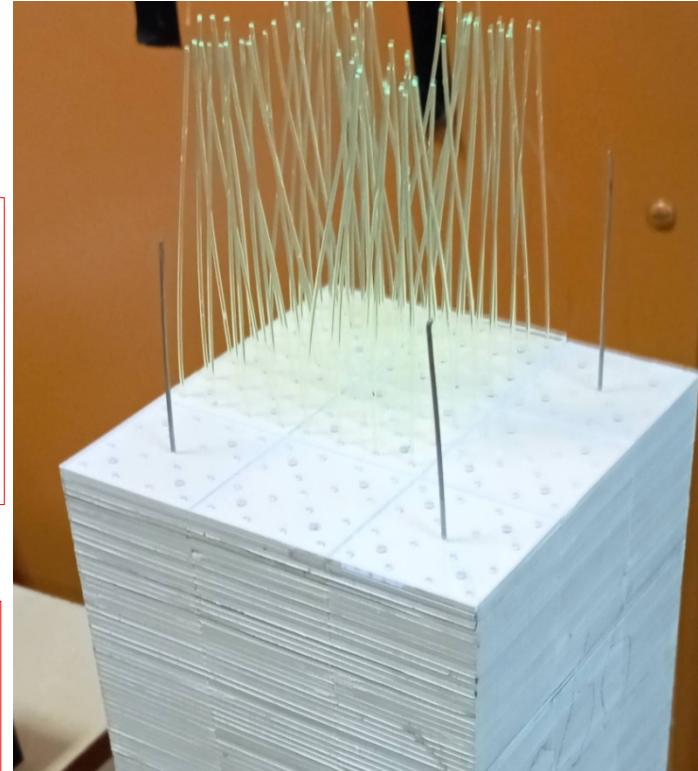


Single Ecal module shown in assembling stage.
It is visible 9 cells as 3x3 matrix with WLS fibers (16 per cell). Y11(200) diameter 1.0 mm was used.

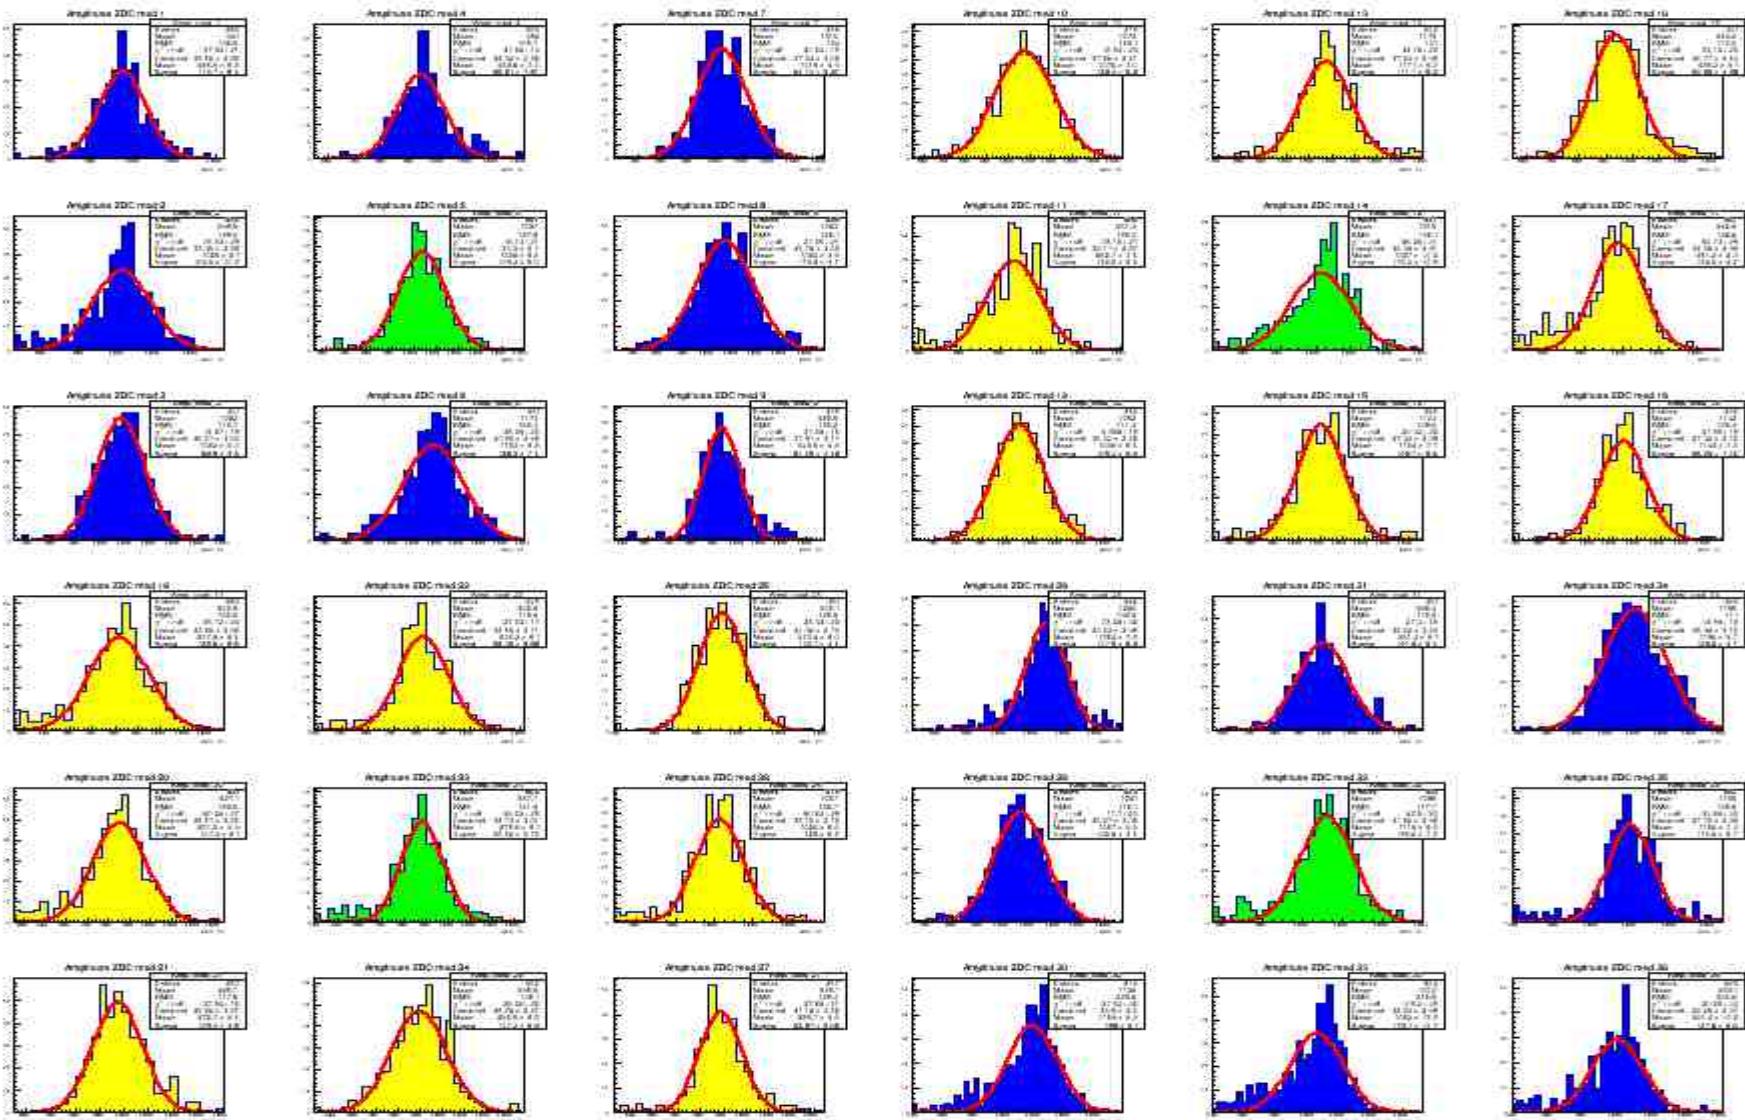


MIP spectra from 36 Cells. Top view shown on picture Above. One hit/event – applied selection criteria during analysis.
 10/24/2023 Oleg Gavriishuk, JINR, Dubna , Russia
 Calibration coefficients were found and normalized to 240 MeV.

Sum ECAL Energy

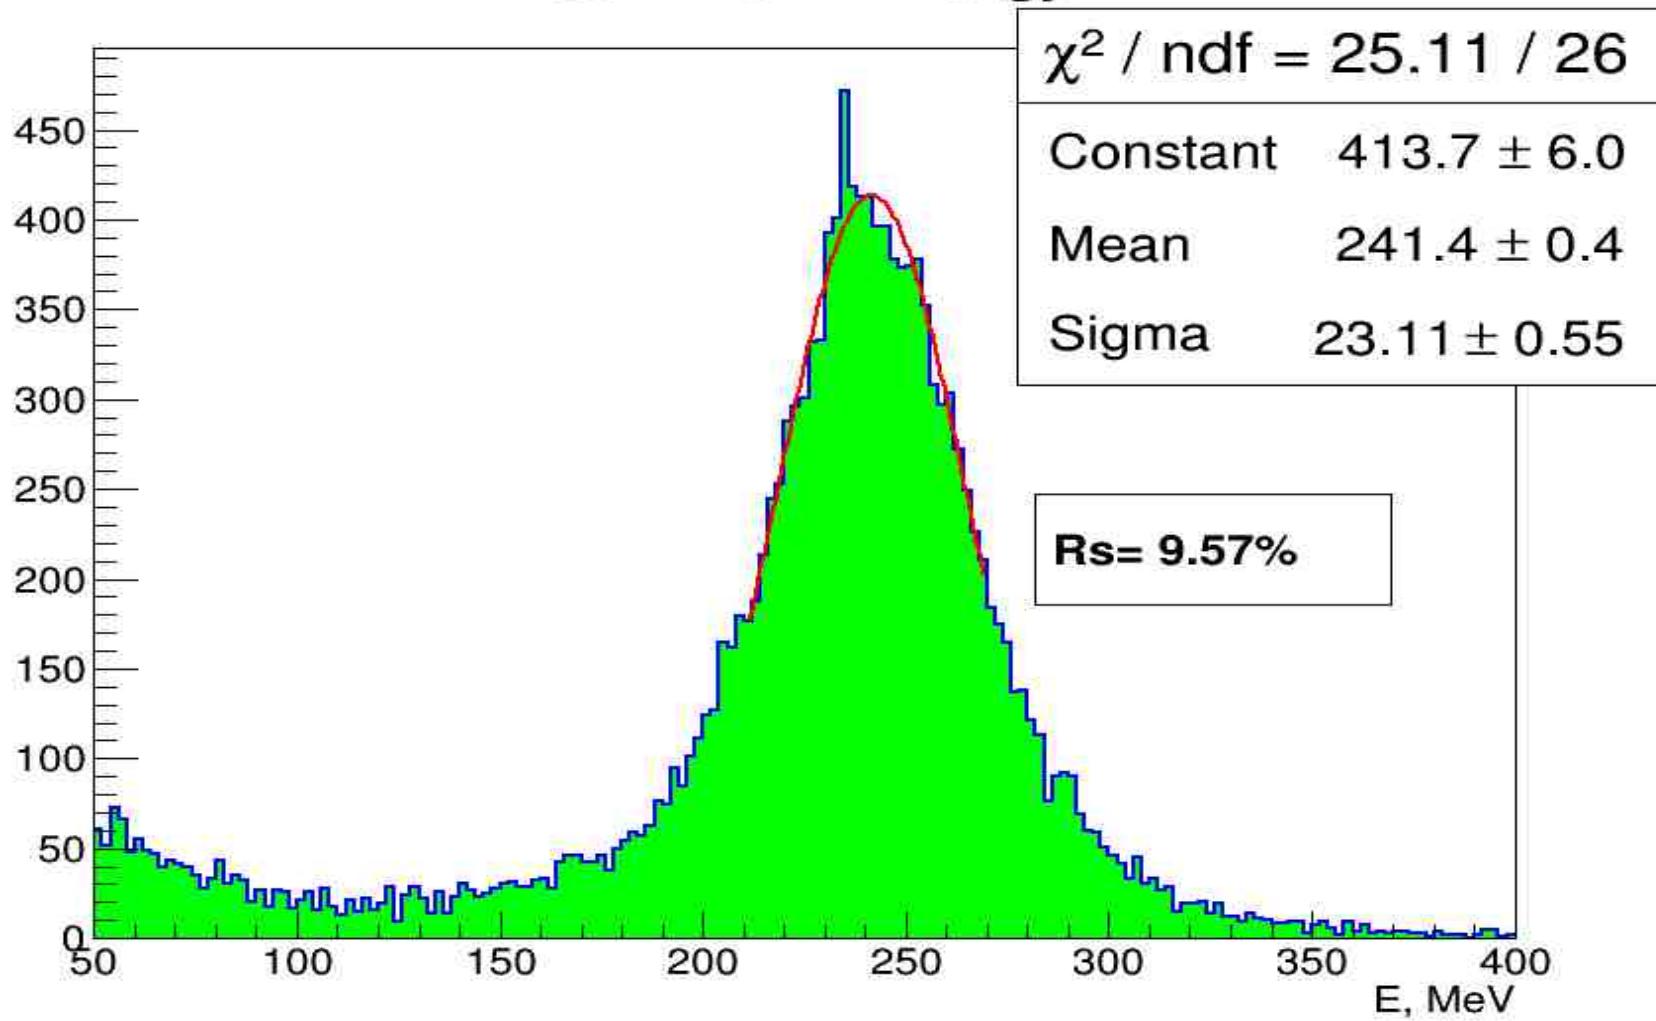


MIP spectra from 36 Cells as Total Sum take in account the Calibration coefficients normalized to 240 MeV. These Energy resolution corresponded to MC

Profile_LED_1_vs_Evt_with_Temp_compensation

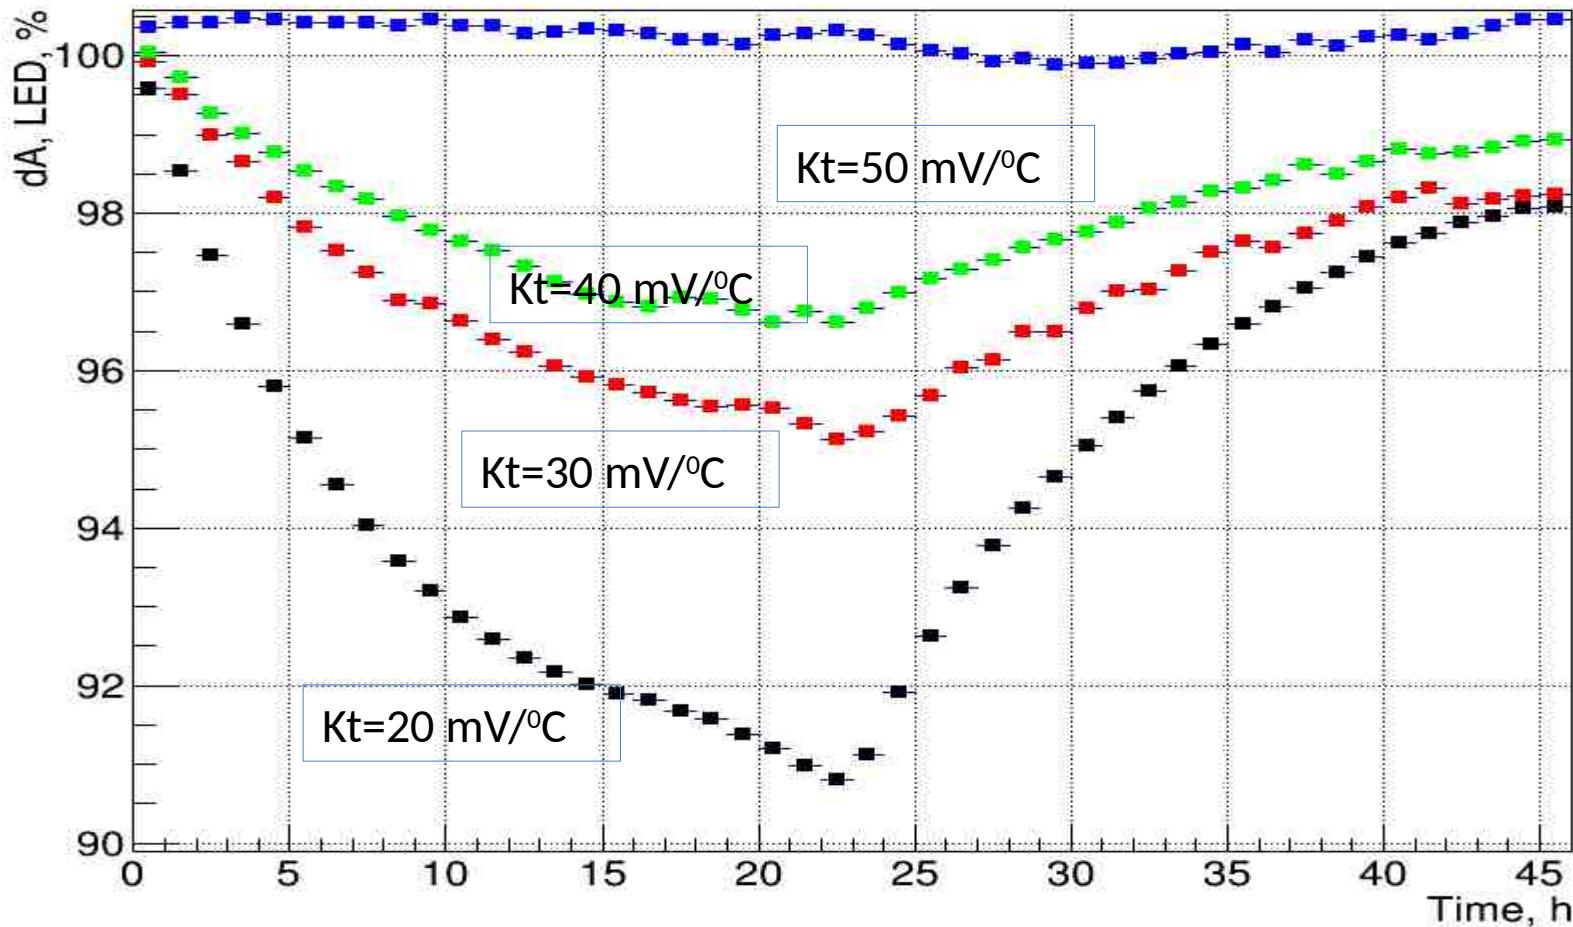


Test of long time Stability was done with different K_t for individual module.
The temperature variation from 20 to 30 $^{\circ}\text{C}$ per day was applied.

Profile_LED_1_vs_Evt

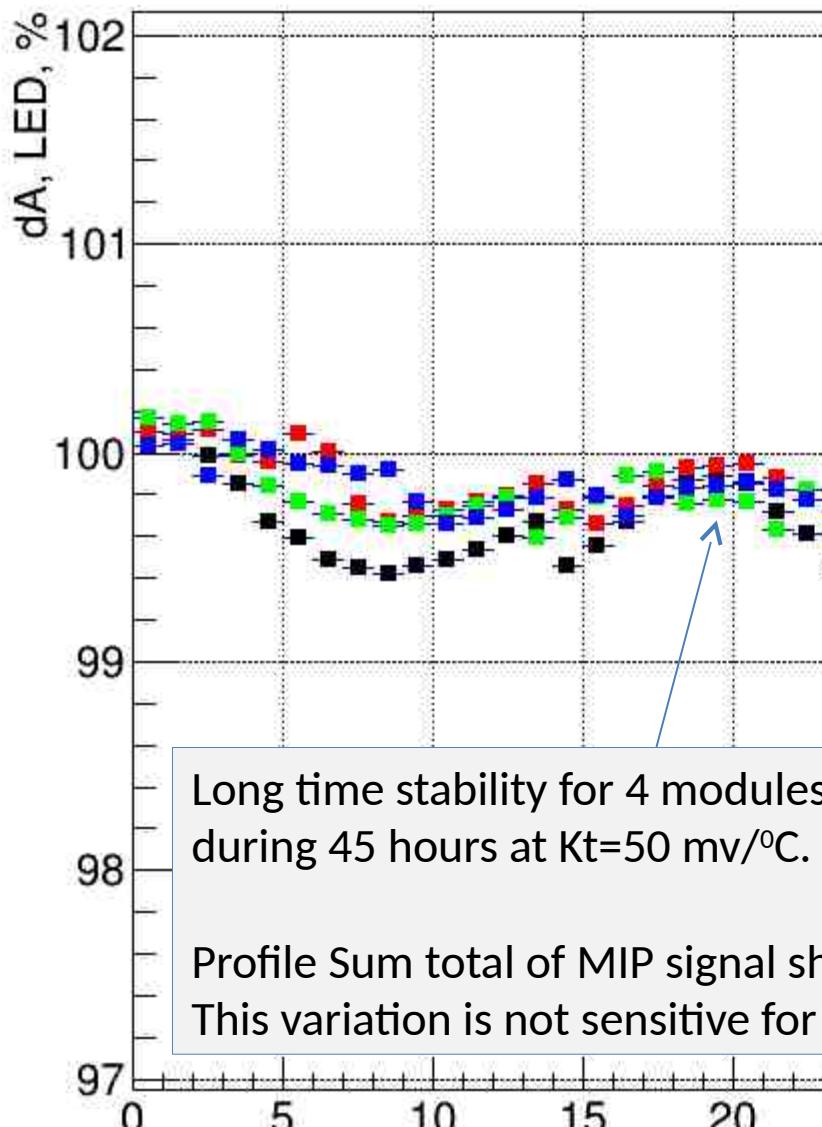

Profile_Sumtot_vs_Evt

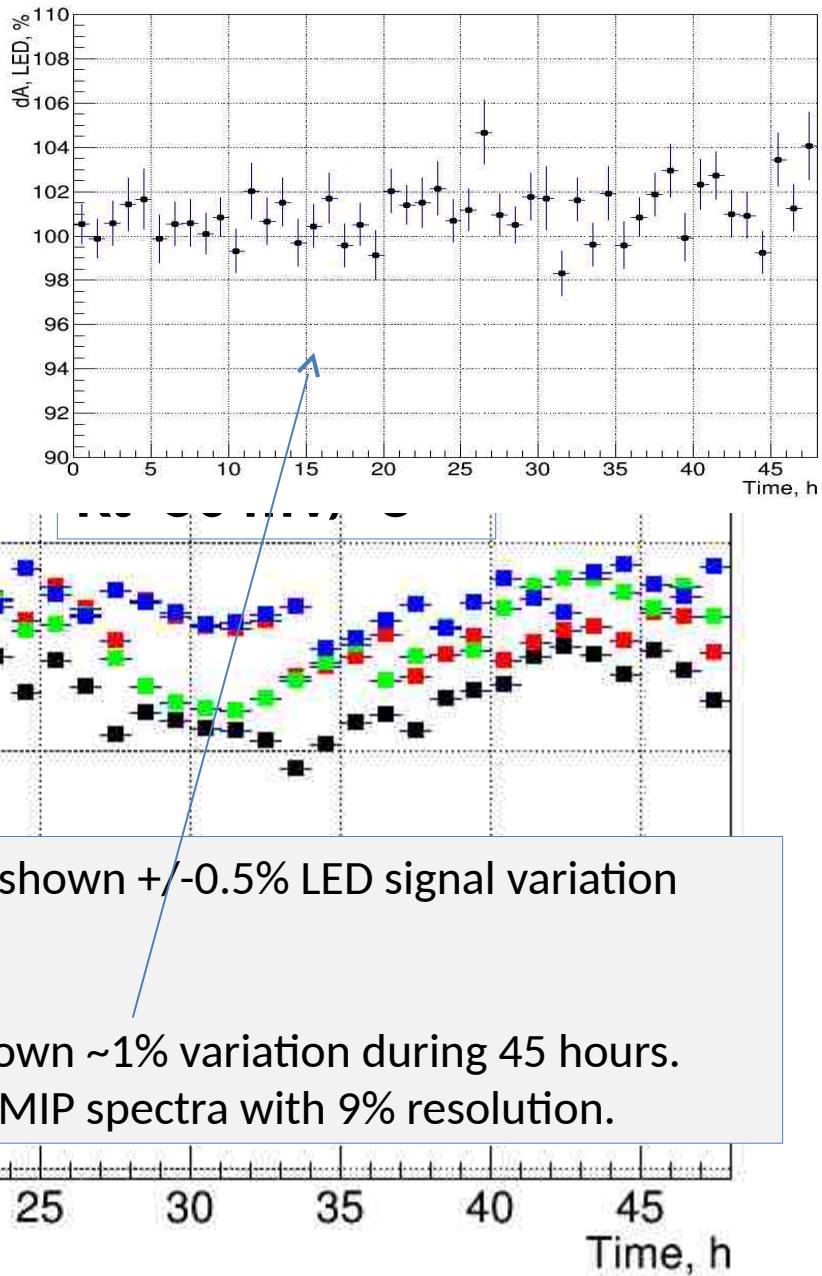

NDL SiPm Series EQR15

11-6060D-S

www.ndl-sipm.net/PDF/Datasheet-EQR15.pdf

NDL (Novel Device Laboratory, Beijing) <http://www.ndl-sipm.net/indexeng.html>

NDL SiPm Series EQR15

11-6060D-S

www.ndl-sipm.net/PDF/Datasheet-EQR15.pdf

- For a conventional SiPM, the quenching resistors are usually fabricated on the surface, and used to connect all APD cells to trace metal lines. In contrast, NDL SiPM employs intrinsic epitaxial layer as the quenching resistors (EQR), and uses a continuous silicon cap layer as an anode to connect all the APD cells. **As a result, the device has more compact structure and simpler fabrication technology, allows larger micro cell density (larger dynamic range) while retaining high photon detection efficiency (PDE).**
- Для обычного SiPM гасящие резисторы обычно изготавливаются на поверхности и используются для соединения всех ячеек APD с металлическими линиями. Напротив, NDL SiPM использует собственный эпитаксиальный слой в качестве гасящих резисторов (EQR) и использует непрерывный слой кремния в качестве анода для соединения всех ячеек APD. **В результате устройство имеет более компактную структуру и более простую технологию изготовления, позволяет увеличить плотность микроячеек (больший динамический диапазон) при сохранении высокой эффективности детектирования фотонов (PDE).**
- NDL (Novel Device Laboratory, Beijing) <http://www.ndl-sipm.net/indexeng.html>



EQR15 Series SiPMs

Specifications subject to change without notice





Type	EQR15 11-1010D-S	EQR15 11-3030D-S	EQR15 11-6060D-S	EQR15 22-1313D-S
Effective Pitch	15 μm			
Element Number	1×1		2×2	
Active Area	1.0×1.0 mm²	3.0×3.0 mm²	6.0×6.0 mm²	1.3×1.3 mm²
Micro-cell Number	4444	40000	160000	7396
Typical Breakdown Voltage (V _B)	30 V			
Temperature Coefficient for V _B	28 mV/°C			
Recommended Operation Voltage	V_B + 8 V			
Peak PDE @ 420nm	45 %			
Gain	4.0×10^5			
Dark Count Rate (DCR)	250 kHz / mm²			
Terminal Capacitance	5.6 pF / mm²			

Above parameters is measured at their recommended operation voltage and 20 °C, and it can operate at 77 K.



EQR15 Series SiPMs

Specifications subject to change without notice

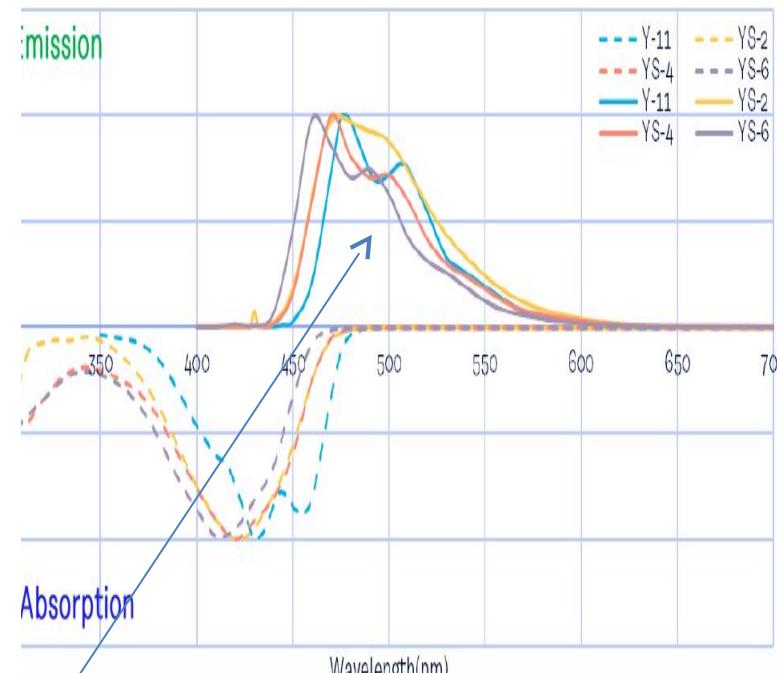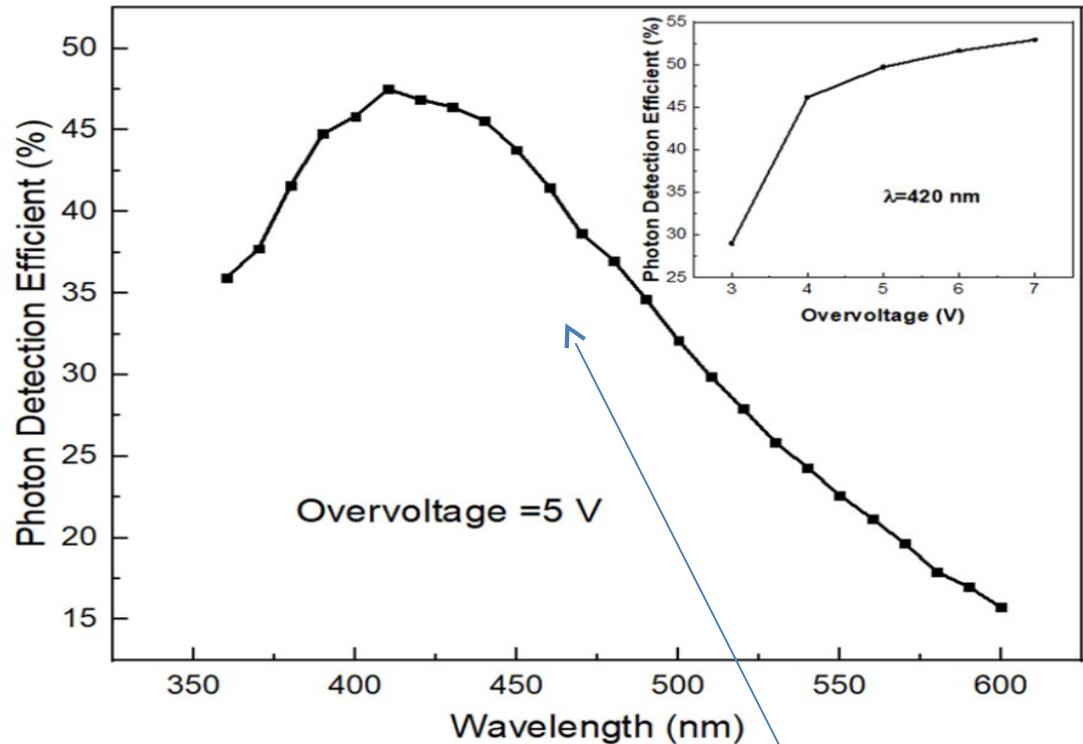

Photon Detection Efficient (PDE) correspond to WLS Emission spectra of Y11.
PDE close to flat maximum about 45% at 6-7 Overvoltage.




EQR15 Series SiPMs

Specifications subject to change without notice




Pulse shape of SiPm with 15 μ pitch and 6x6 mm² size

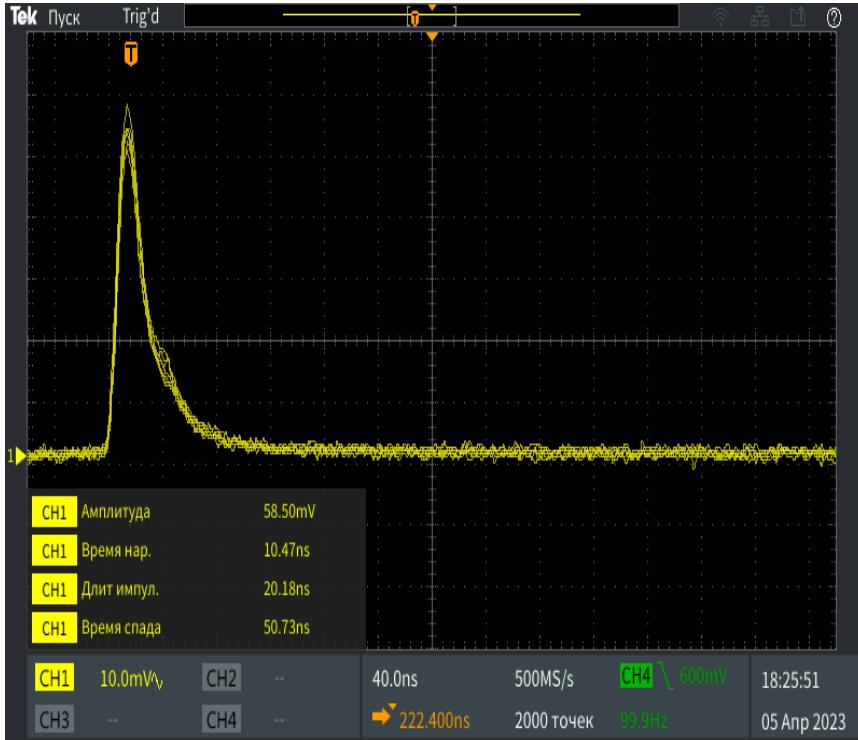

EQR-15-60
Front - 10 ns
Length - 20 ns

10/24/2023







Oleg Gavriishuk, JINR, Dubna , Russia

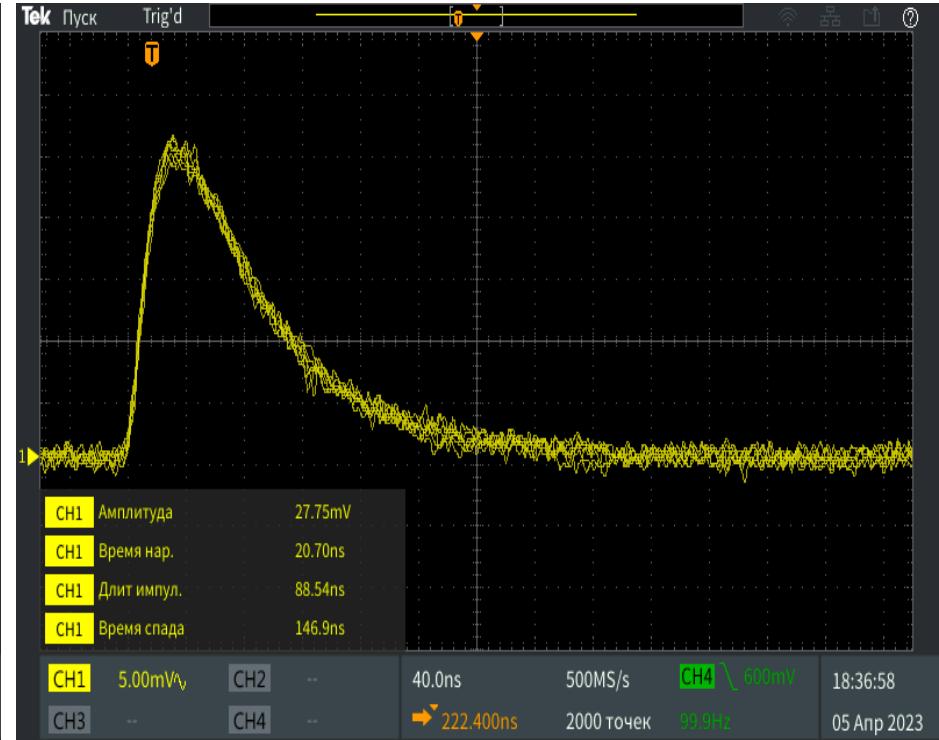



HAMAMATSU S14160-6015
Front - 21 ns
Length - 89 ns

SiPm test Results

- Dark Current measurements
- Gain vs Overvoltage: dA/dU
- Gain vs Temperature: dA/dt
- PDE vs Overvoltage
- Operation Volt. how to select it
- Temperature stability studies

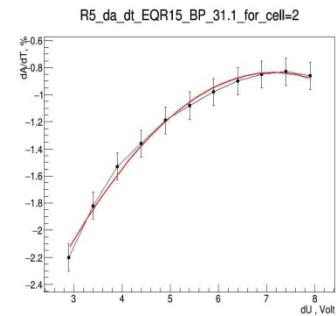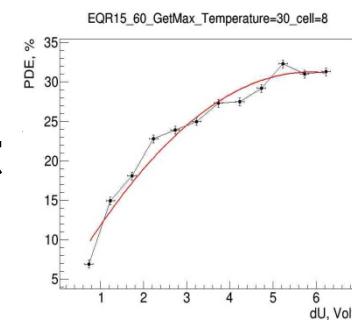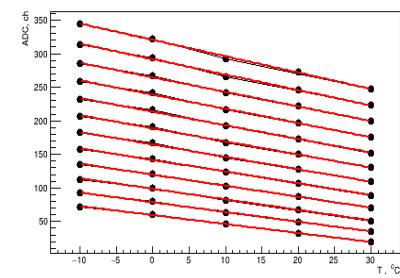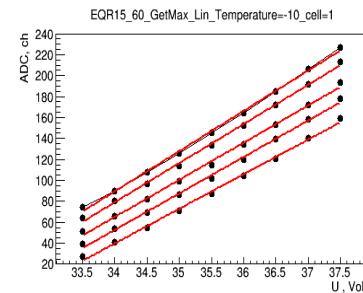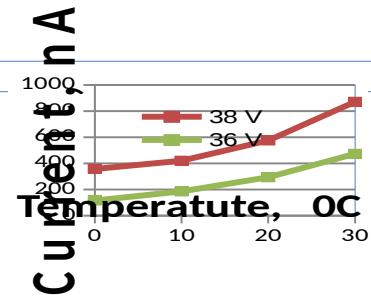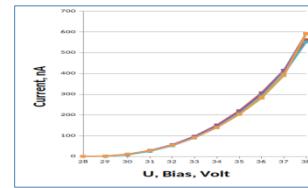


EQR15-60 Dark Current vs Bias voltage and its temperature dependences around operate Voltage

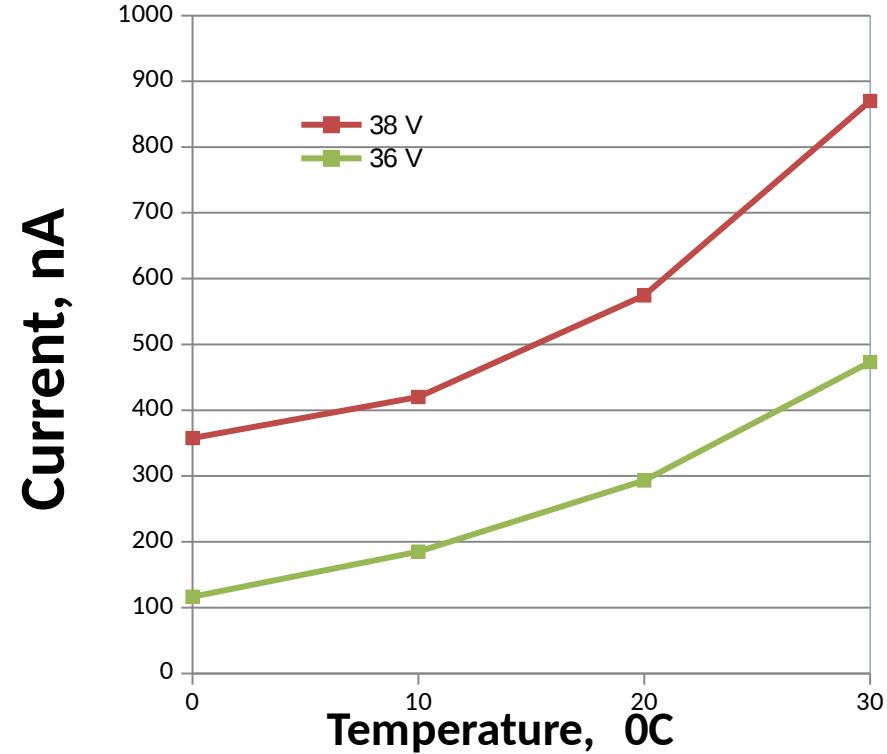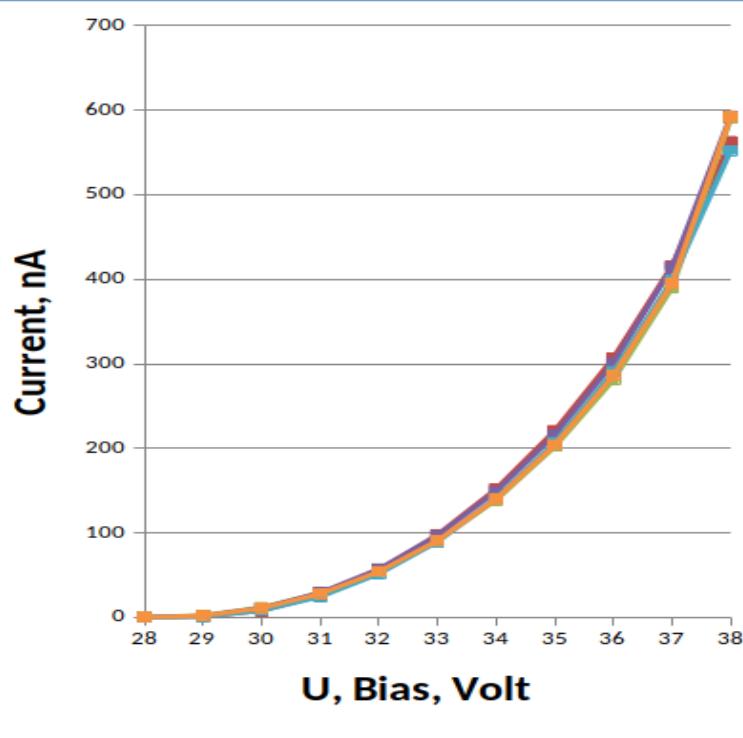


Dark Current vs Operation Bias (36-37 V) at room temperature (20°C) is equal to 300-400 nA. Its are corresponded to the factory data and is similar HAMAMATSU too.

Gain vs Overvoltage allow obtain:
 $\text{slope} = dA/dU$ vs U

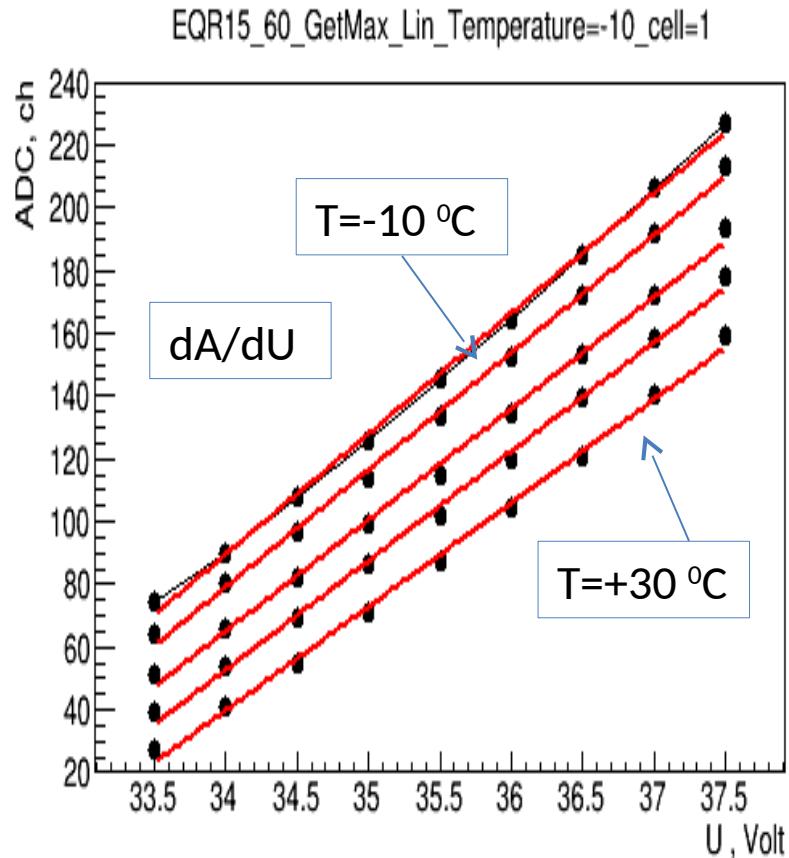


Gain vs Temperature allow obtain:
 $\text{slope} = dA/dT$ vs T

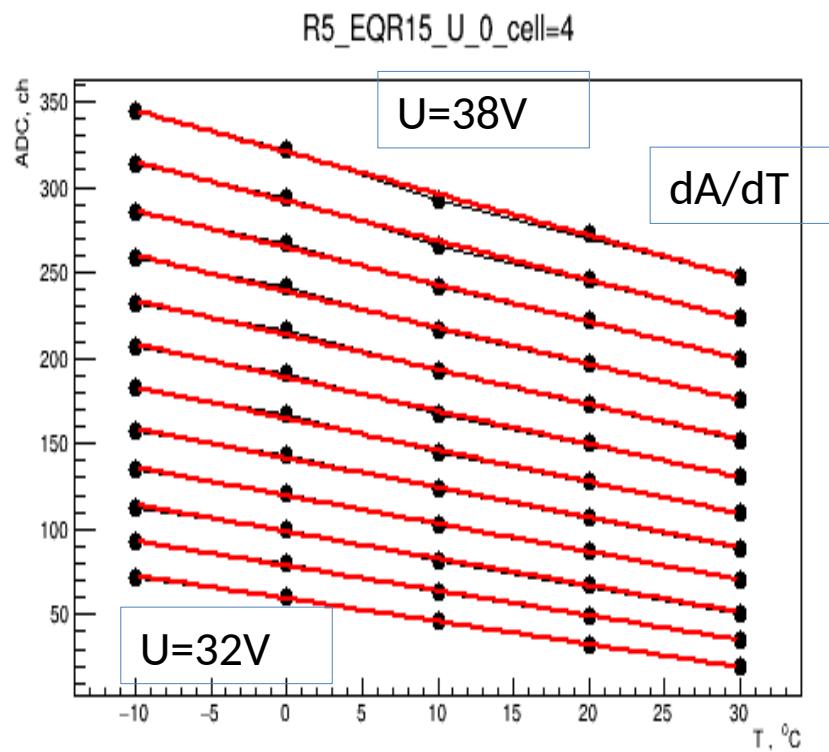


$$K_t = dU/dT = dA/dT / dA/dU$$

The thermal stabilization coefficient (K_t) was defined as the ratio of the slope dA/dT to the slope dA/dU depending on the applied bias.

Break Point (Bp) was defined as extrapolation point of dA/dU to zero. Take assumption his linear behavior from Temperature we find that $Bp=32$ V at 20°C .

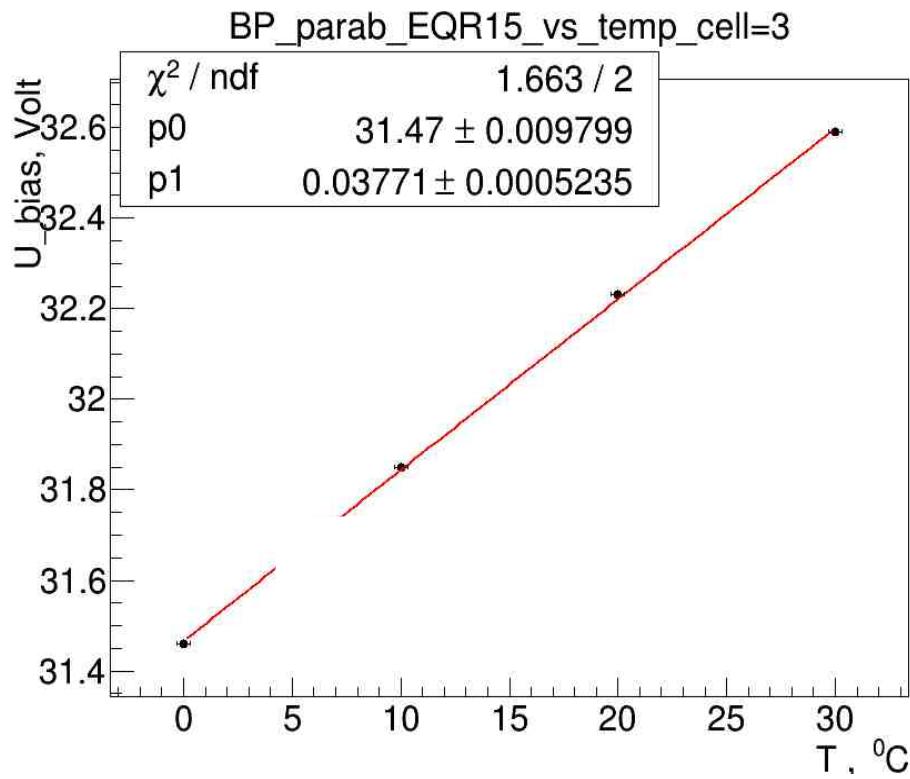

$Kt=dU/dT=dA/dt/dA/dU$ fom previous slides we find that dependence from Overvoltage has linear behavior and equal to $\sim 50 \text{ mV/}^{\circ}\text{C}$ at Operation point 5.5 V.

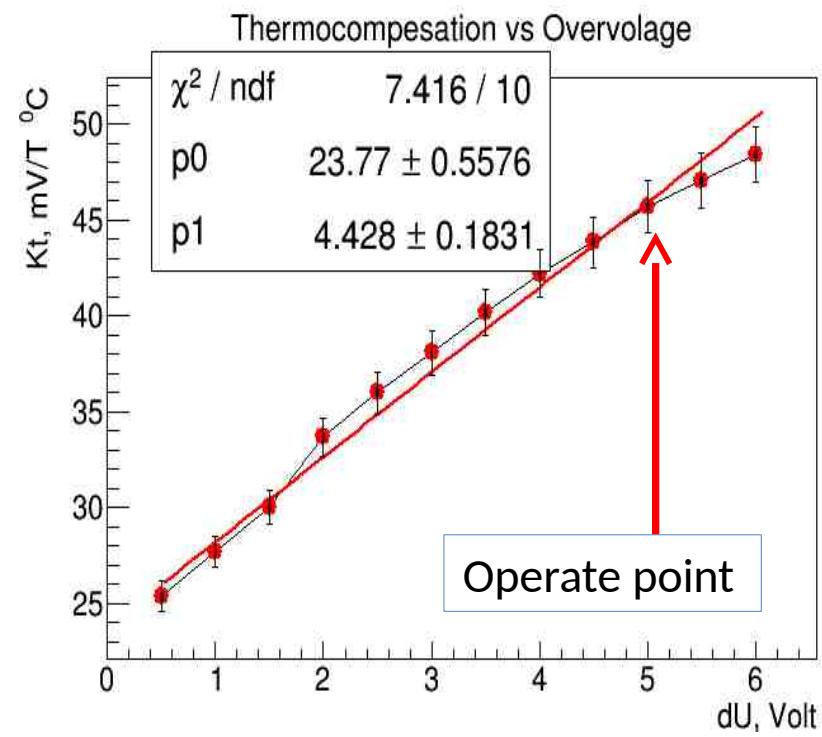


Temperature sensitivity vs dU

Photon Detection Efficient vs dU


dA/dT vs dU

R5_da_dt_EQR15_BP_31.1_for_cell=2

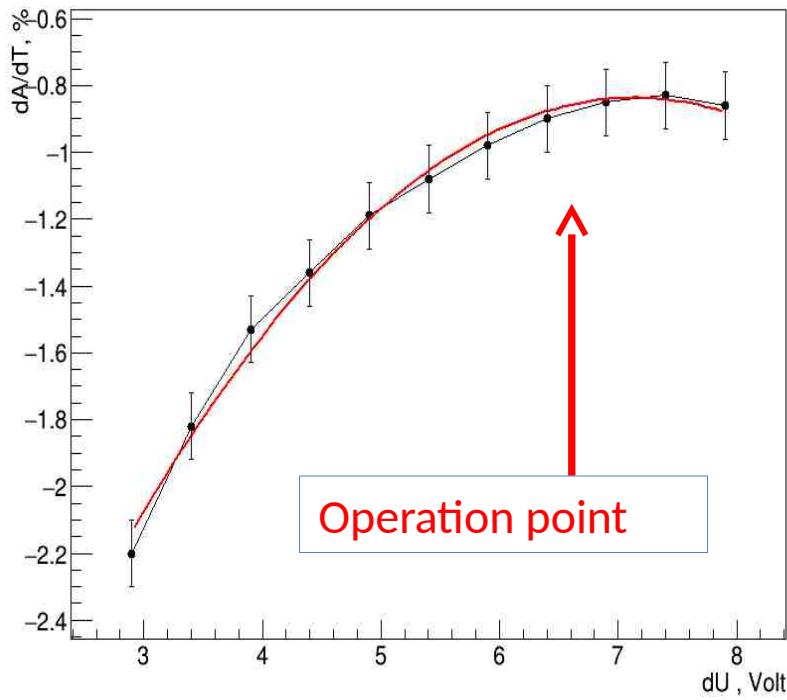

PDE vs dU

EQR15_60_GetMax_Temperature=30_cell=8

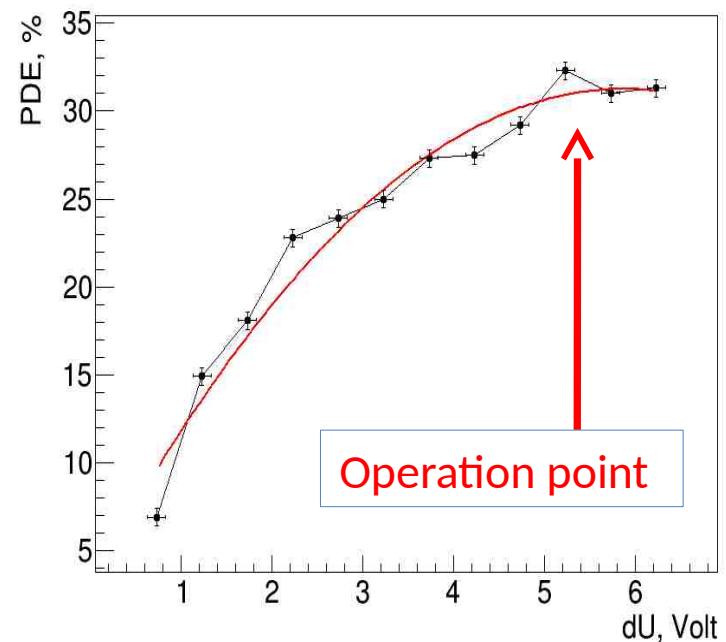


Operation point was found at **dU=6.5 V** take in account that:

1. dA/dT and PDE - has Plato in dU.
2. dA/dT has minimal value ~ 1%/°C , PDE close to maximal value ~ 32%.




Matrix form drawing 2023 for scintillator production (40x40x1.5 mm³)

Shown t drawing of 4 sets form to produce 4 scintillator plates per one cycle.
Matrix form it is a special setup for molding by pressure technology.

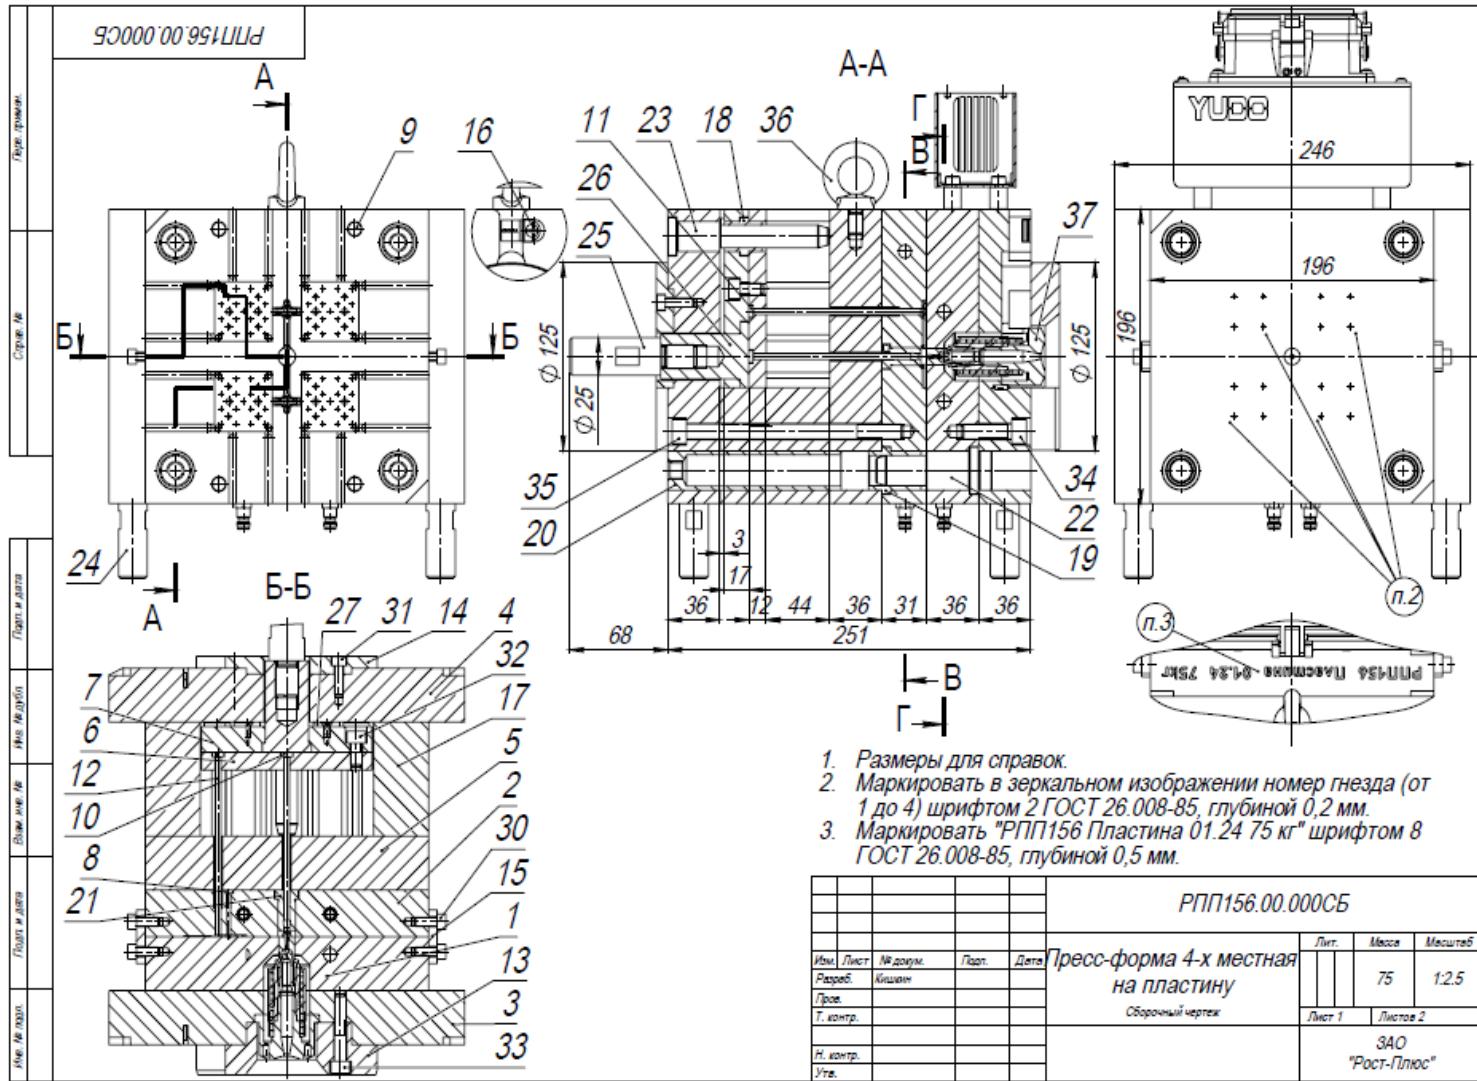


4-Set Matrix form for scintillator production

Matrix form is special setup for molding by pressure technology.
It allow produce the scintillators from granulated polystyrene with dopants.
4 set form produce 4 scintillators plates of $40 \times 40 \times 1.5 \text{ mm}^3$ per 1 minute.

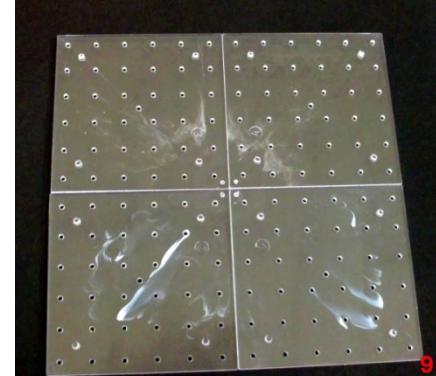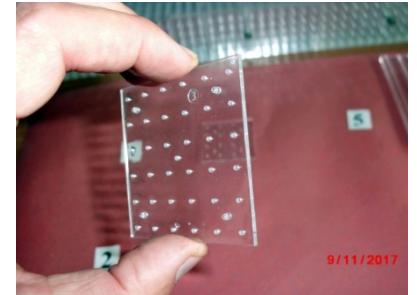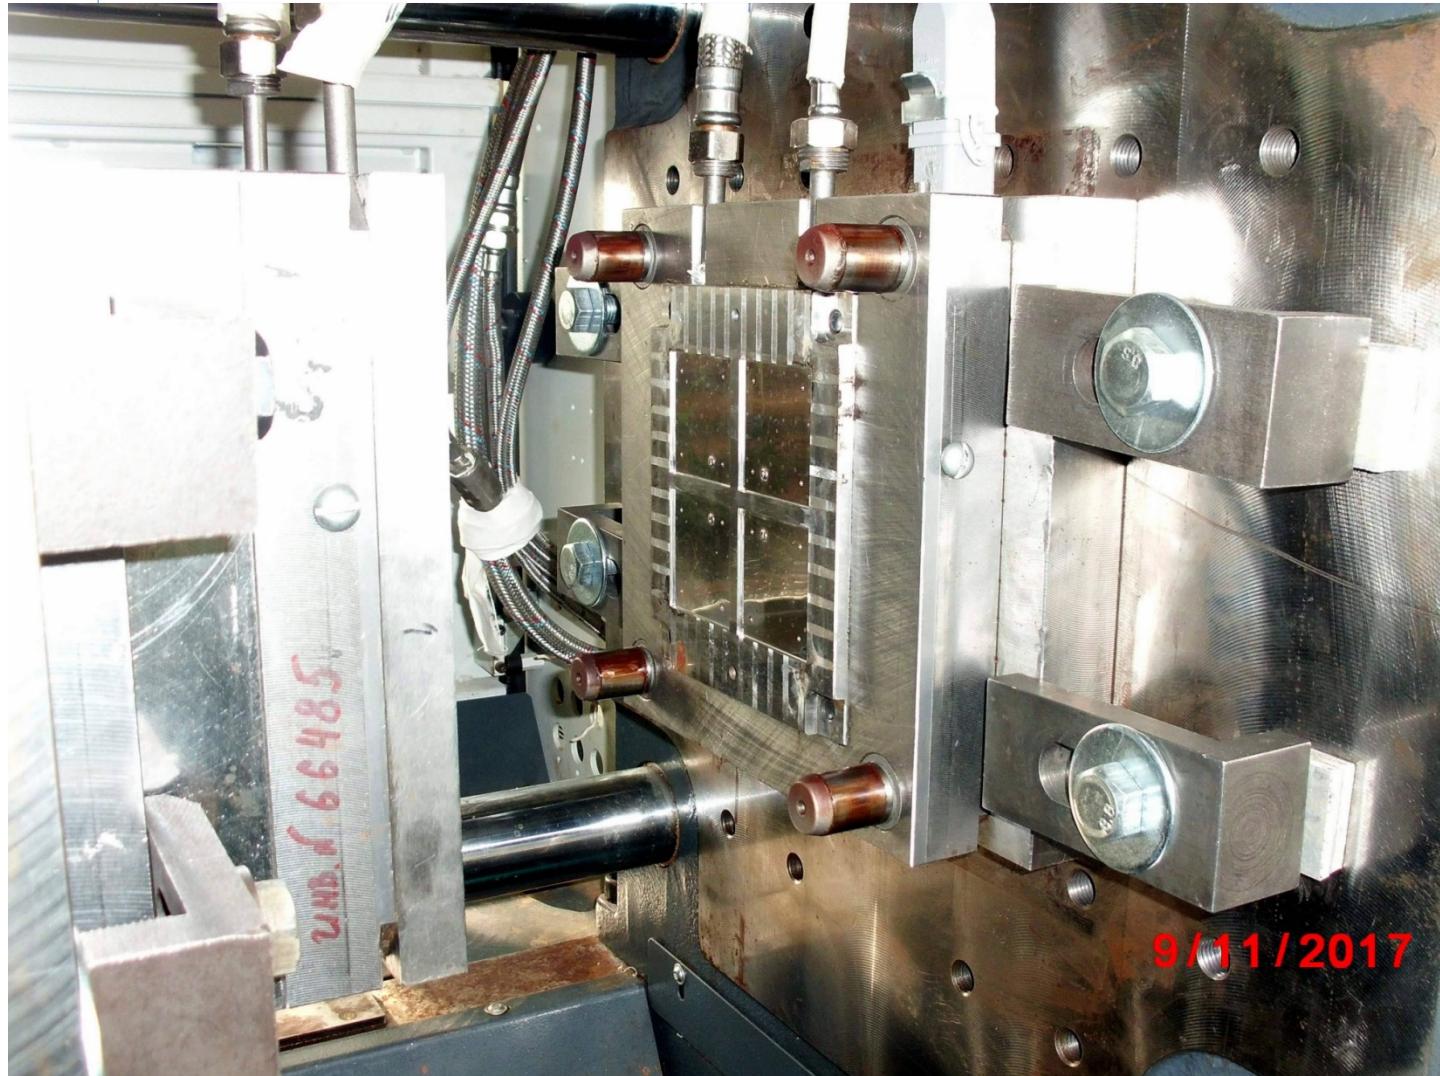

End Cup for SPD with new scintillator to be produced in 2024 via 256 cells of 40x40 mm²

It is I-st stage possible setup to estimate the particles flow at NICA

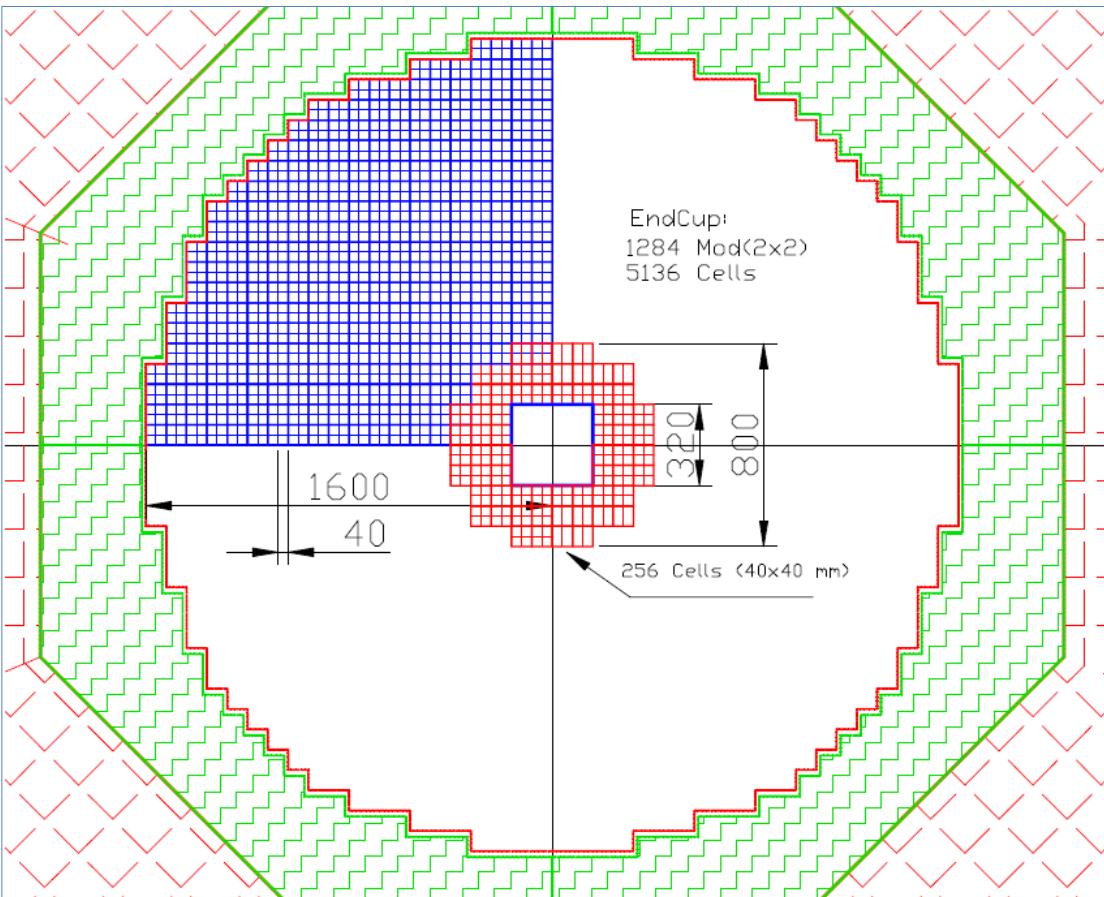


This Figure shows in red 64 modules, consisting of 4 cells each. The weight of this assembly is 597 kg. This will require 130 kg of polystyrene, 465 kg of lead, as well as additives: 1.95 kg of P-terphenyl and 65 g. POPOP, and 2000 meters WLS fiber type Y-11.

It is 1/20 part of End Cup and taken time of 36 Days to prepared 51200 Stint. plates.


To read this setup, we need four ADC64 - 64-channel amplitude encoders, as well as 16 boards of 16-channel amplifiers and bias voltage regulators.

End Cup for SPD with new scintillator to be produced in 2024 via 256 cells of $40 \times 40 \text{ mm}^2$

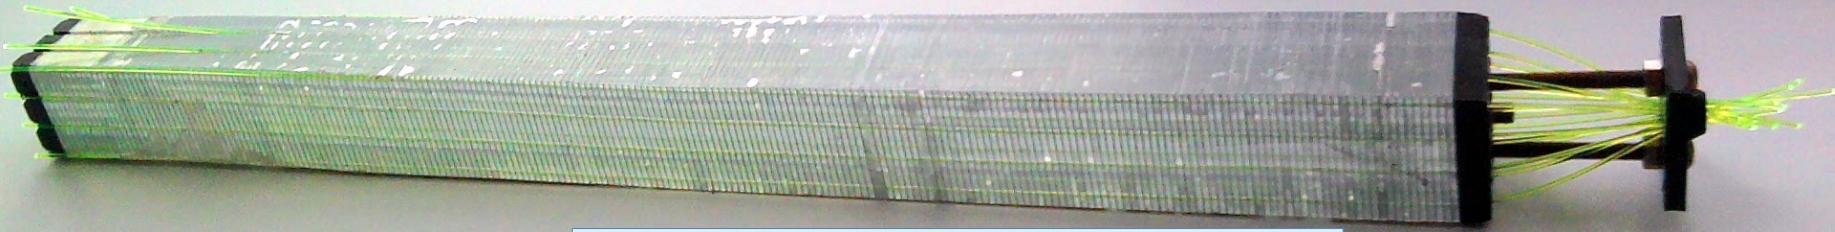


Single Cell $40 \times 40 \text{ mm}^2$

One Module setup consist from 4 cells of 2×2

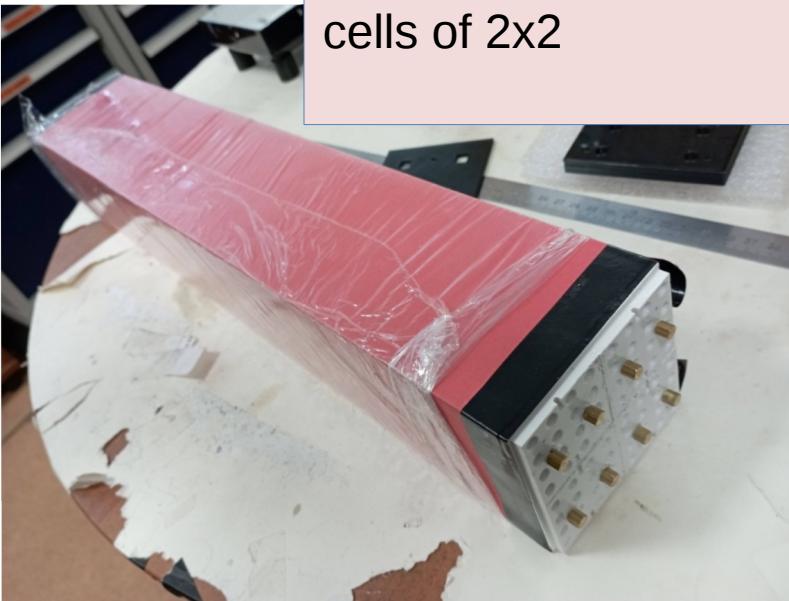

In red is shown 64 Modules, consisting from 4 cells each of 2×2 .

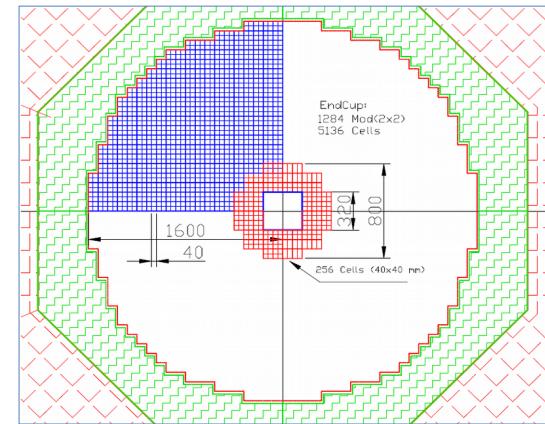

Conclusions

1. New ECAL geometry was designed in 2023
2. SiPm EQR15-60 China production were studied
3. New ECAL setup with cell size $4 \times 4 \text{ cm}^2$ assembled
4. ECAL test in cosmic rays was done
5. Matrix form for new scintillator production
should be ready in end of 2023
6. New scintillator production will start in beginning
of 2024

70 лет ЛФВЭ



NICA
2023

ЭФЛАН 1953 -
ЛВЭ 1956

End of Report

Thanks for attention to All