
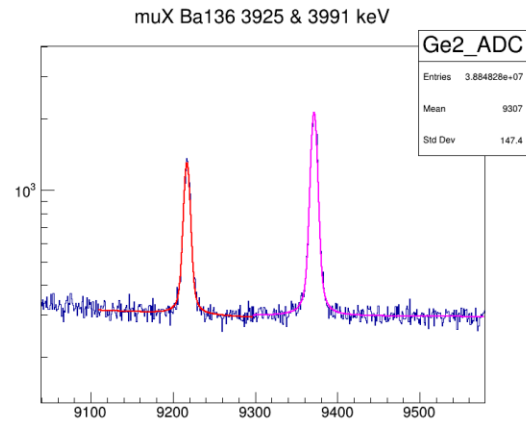
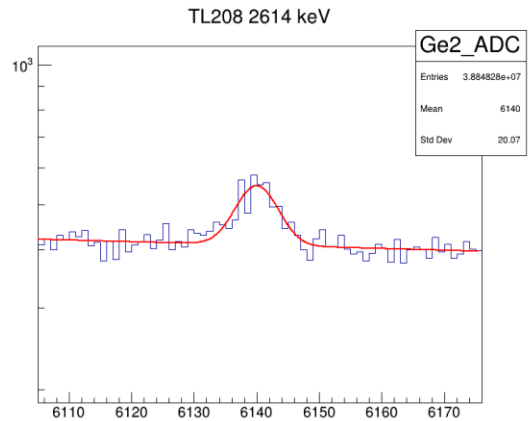
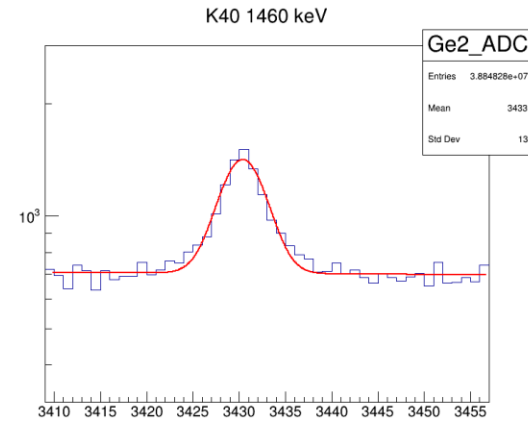
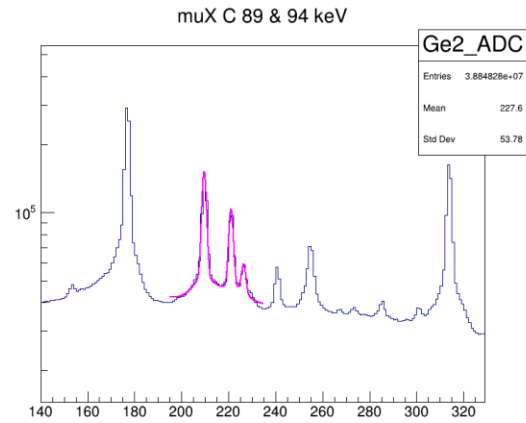



MIDAS. Ge02 (Ch.1) energy calibration

Igor Zhitnikov
MONUMENT@2023-06-16


Lines for regular calibration during Ba-136 measurements

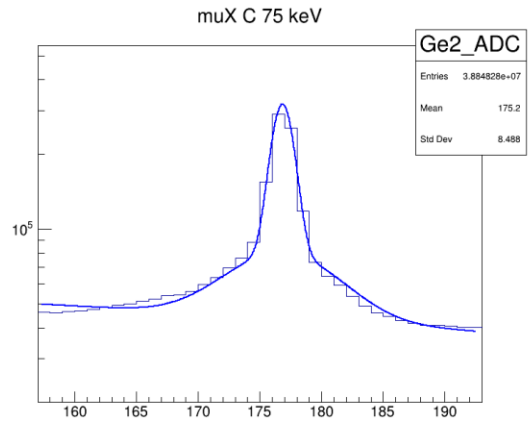

Calibration with radioactive sources + muX Pb-208

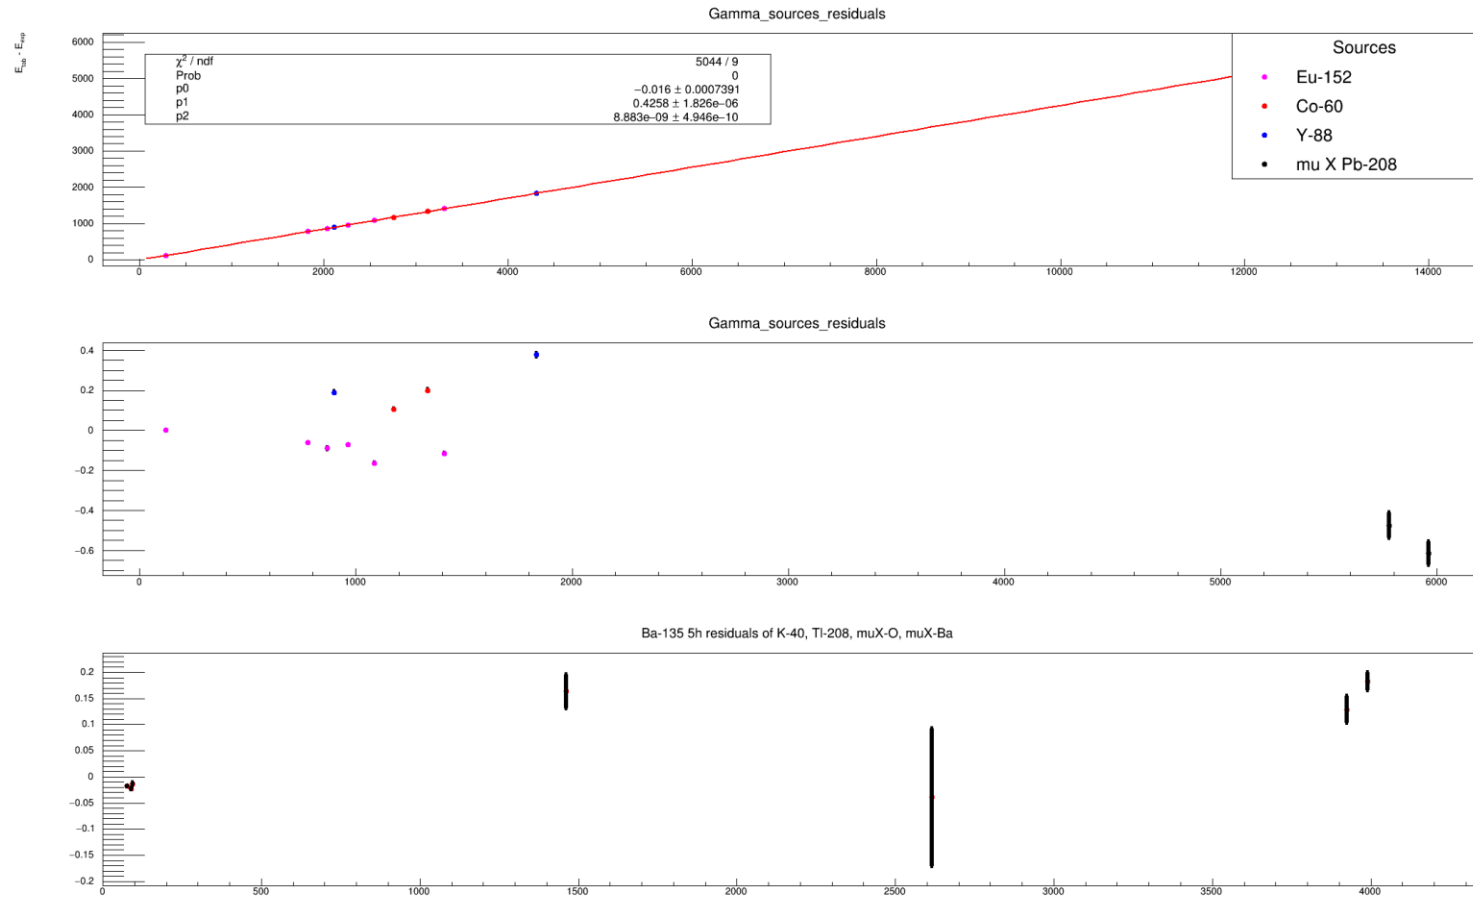

Calibration with muX O, muX Ba-136, K-40 and Pl-208 lines

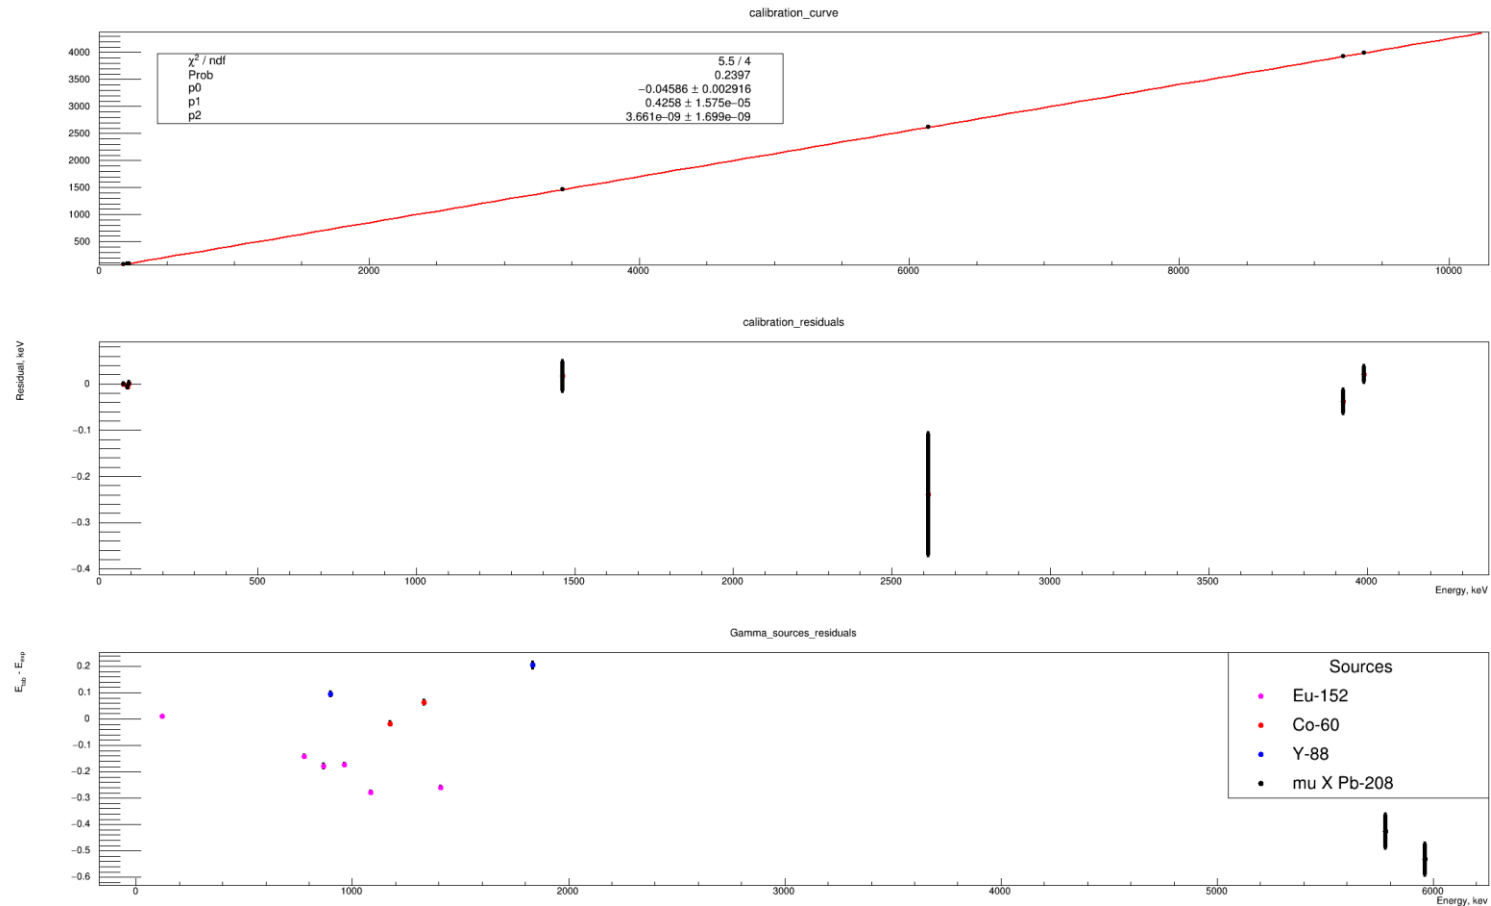

Calibration with Eu-152 + muX Pb-208

