

# Stilbene-based neutron TOF-spectrometer


Anh Mai

ACCULINNA group,  
Flerov Laboratory of Nuclear Reactions

60<sup>th</sup> meeting of the PAC for Nuclear Physics  
23 January 2025, JINR



# Main areas of interest at FLNR at nuclide chart

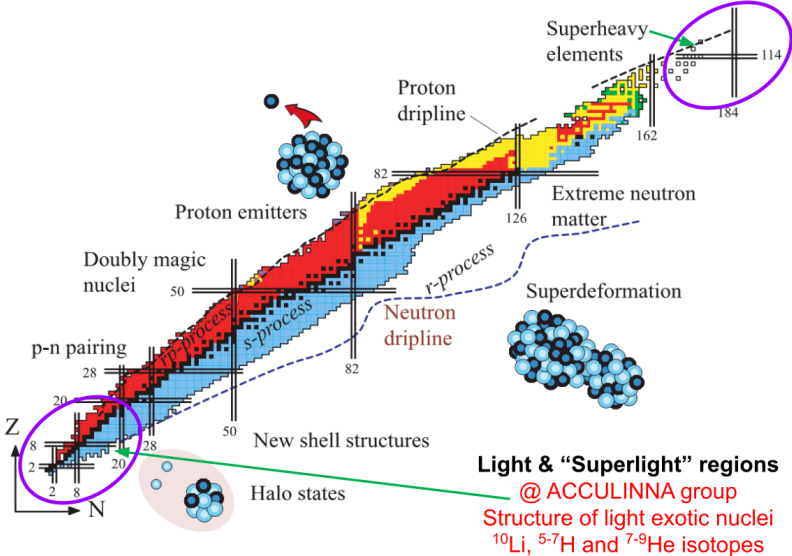

# Motivation


	Li 4 91 ys	Li 5 370 ys	Li 6 7.59	Li 7 92.41	Li 8 839.40 ms	Li 9 178.3 ms	Li 10 2.0 zs	Li 11 8.75 ms	Li 12 <10 ns	Li 13 3.3 zs	
2	He 3 0.000134	He 4 99.999866	He 5 700 ys	He 6 806.92 ms	He 7 2.51 zs	He 8 119.1 ms	He 9 2.5 zs	He 10 3.1 zs			10
	H 1 99.9885	H 2 0.0115	H 3 12.32 y	H 4 139 ys	H 5 >910 ys	H 6 290 ys	H 7				8
		n 1 613.9 s	2	4	6						

Measurement of correlations,  
⇒ detection of **neutrons** in coincidences with  
charged reaction products is needed.

# Motivation

	Li 4 91 ys	Li 5 370 ys	Li 6 7.59	Li 7 92.41	Li 8 839.40 ms	Li 9 178.3 ms	Li 10 2.0 zs	Li 11 8.75 ms	Li 12 <10 ns	Li 13 3.3 zs
2	He 3 0.000134	He 4 99.999866	He 5 700 ys	He 6 806.92 ms	He 7 2.51 zs	He 8 119.1 ms	He 9 2.5 zs	He 10 3.1 zs		
H 1 99.9885	H 2 0.0115	H 3 12.32 y	H 4 139 ys	H 5 >910 ys	H 6 290 ys	H 7				
	n 1 613.9 s	2	4	6						

Measurement of correlations,  
 $\Rightarrow$  detection of **neutrons** in coincidences with charged reaction products is needed.

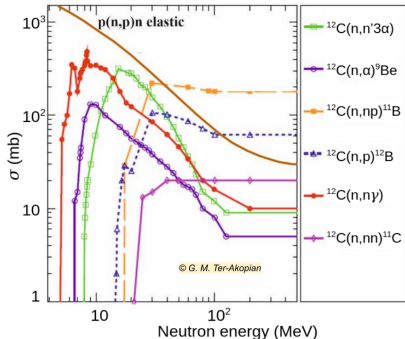

Neutron-matter interaction cross-sections  
 in accordance with different neutron energies

## Stilbene crystals:

- high luminescence efficiency
- fast response time
- crystalline and solid  
 $\rightarrow$  high durability, non-flammable
- greatly sensitive to neutrons  
 $\rightarrow$  well-suited in our range
- excellent **n -  $\gamma$  discrimination**

$\Rightarrow$  Stilbene was implemented @ ACCULINNA-2.

# Stilbene based neutron spectrometer




- unsettled incident neutron energy  
- scintillator response correlation  
→ TOF method is applied,
- undesirable  $\gamma$ -background  
→  $n - \gamma$  separation performance,
- light output is non-linear and different for diverse particles,
- neutron registration efficiency

The neutron spectrometer assembly @ ACCULINNA-2

⇒ The characterization of neutron TOF spectrometer, where amplitude and time resolution,  $n - \gamma$  discrimination, light output response and detection efficiency were investigated.

# 1. Gamma measurements

# Amplitude calibration

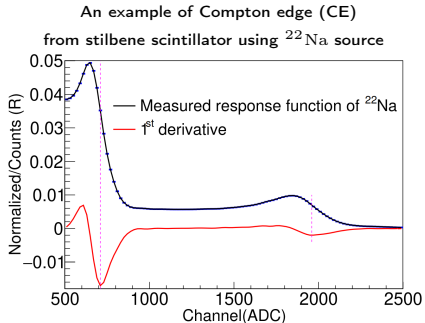


$$E_{CE} = E_{\gamma} \left( 1 - \frac{1}{1 + \frac{2E_{\gamma}}{m_e c^2}} \right)$$

⇒ 1st derivative of measured response  
combined with GEANT4 simulation  
for precise CE determination

# Amplitude calibration




An example of Compton edge (CE)

from stilbene scintillator using  $^{22}\text{Na}$  source

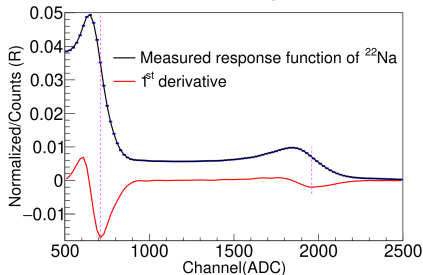

$$E_{CE} = E_{\gamma} \left( 1 - \frac{1}{1 + \frac{2E_{\gamma}}{m_e c^2}} \right)$$


⇒ 1st derivative of measured response combined with GEANT4 simulation for precise CE determination

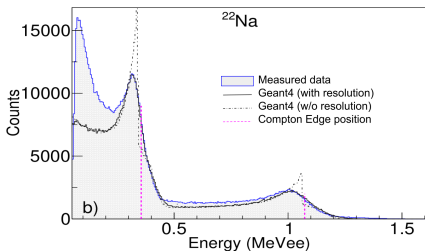



# Time resolution

$\gamma - \gamma$  coincidence measurement

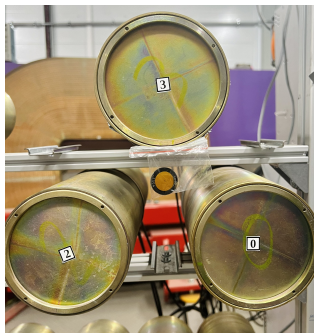


$$\sigma_1^2 = \frac{1}{2}(\sigma_{12}^2 + \sigma_{13}^2 - \sigma_{23}^2)$$

$$\sigma_2^2 = \frac{1}{2}(\sigma_{12}^2 - \sigma_{13}^2 + \sigma_{23}^2)$$

$$\sigma_3^2 = \frac{1}{2}(-\sigma_{12}^2 + \sigma_{13}^2 + \sigma_{23}^2)$$

# Time resolution

$\gamma - \gamma$  coincidence measurement

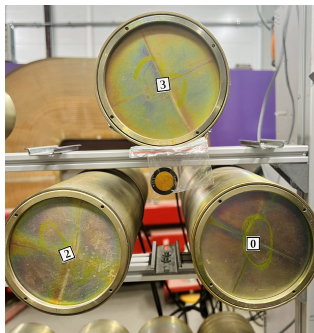


$$\sigma_1^2 = \frac{1}{2}(\sigma_{12}^2 + \sigma_{13}^2 - \sigma_{23}^2)$$

$$\sigma_2^2 = \frac{1}{2}(\sigma_{12}^2 - \sigma_{13}^2 + \sigma_{23}^2)$$

$$\sigma_3^2 = \frac{1}{2}(-\sigma_{12}^2 + \sigma_{13}^2 + \sigma_{23}^2)$$

Time resolution relies upon the amplitude signal

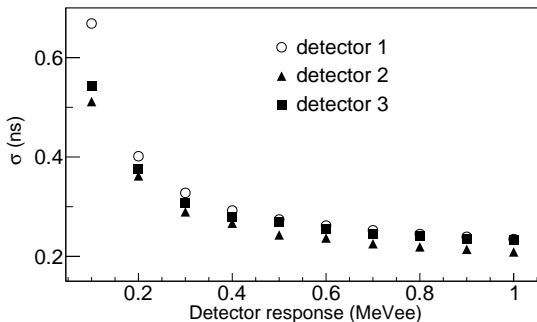

→ different range of data derives from disparate signal sizes,


→ low-energy events are associated with the registration of rescattered  $\gamma$ -quanta.

## 2. Neutron measurement


# ING-27 DT neutron generator

The experimental schematic of

DT-reaction

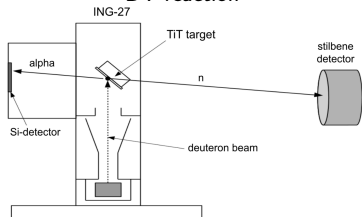

ING-27 dimensions (mm) in experiment

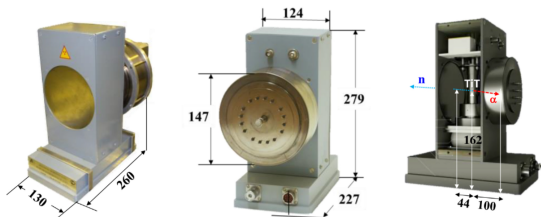


- a deuteron-beam @ 100 keV bombards a thin titanium-tritium TiT target by means of  $d + t \rightarrow \alpha + n$  fusion reaction to produce 14-MeV neutrons,
- the neutron generator has an intensity up to  $10^8$  n/s in  $4\pi$ ,
- $\alpha$ -particles were registered by a 64-pixel ( $8 \times 8$  strip) DSSD @ 100 mm from the target,
- stilbene was placed at a distance of 15 cm for neutron detection.


# Neutron-gamma discrimination

The scintillation process by means of  $\pi$ -electronic

energy levels of an organic molecule




Timing signals for gamma and neutron in the scintillator

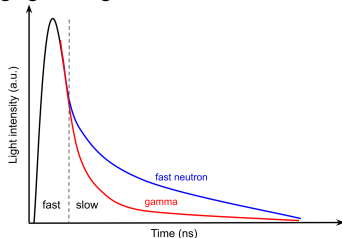

# Neutron-gamma discrimination

The scintillation process by means of  $\pi$ -electronic

energy levels of an organic molecule



Timing signals for gamma and neutron in the scintillator



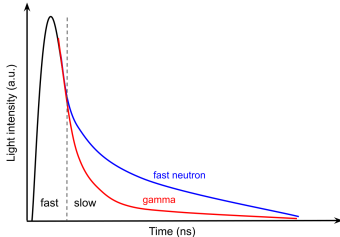



Illustration of neutron-gamma separation by

Pulse Shape Analysis from the 14-MeV neutron generator.

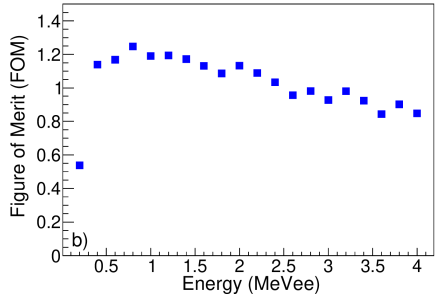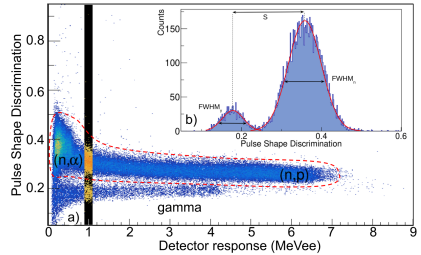


# Light output response in organic scintillator

Neutron interaction with stilbene scintillator  
leads to a large number of different processes

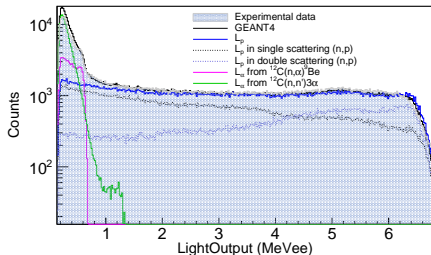


# Light output response in organic scintillator

Neutron interaction with stilbene scintillator leads to a large number of different processes

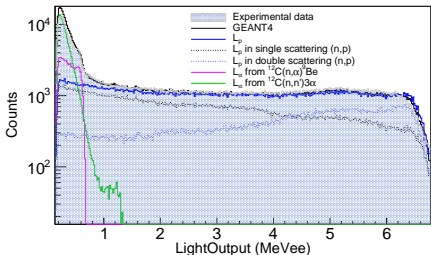

Light output response of stilbene scintillator to protons and alpha particles

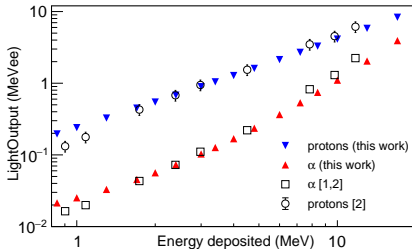

- Chiefly, protons and  $\alpha$ -particles produce the main light in the stilbene detector,
- The response of proton +  $\alpha$ -particles was simulated and reconstructed with measured data, and compared with other works,
- Knowing the proton-response is the key to determine the incoming neutron energy.


[1] V. Verbinski et al., Nucl. Instrum. Methods 65 (1), 8–25 (1968).

[2] R.L. Craun and D.L. Smith, Nucl. Instrum. Methods 80, 239–244 (1970).




# Neutron registration efficiency

The calculated response in the stilbene detector  
to various incident neutron energies

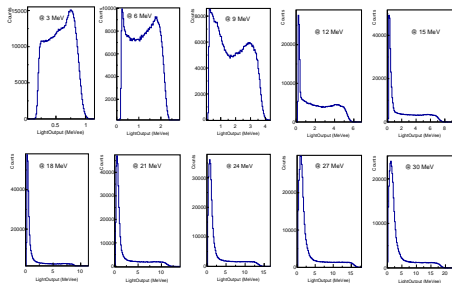


# Neutron registration efficiency

The calculated response in the stilbene detector to various incident neutron energies

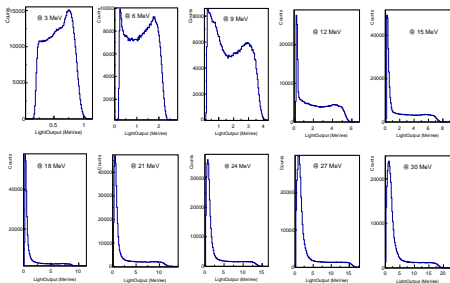

The measured and calculated neutron efficiency in the energy range of 3-30 MeV

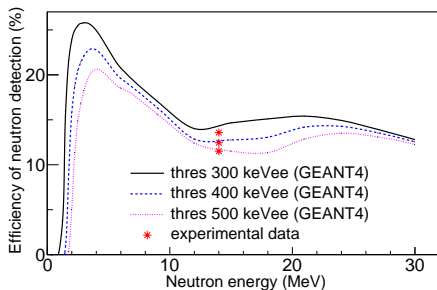

→ Measured data at 14 MeV was compared with GEANT4, thus neutron registration can be estimated in other energy ranges from 3-30 MeV.

# Conclusions

- The performance of stilbene based modular neutron spectrometer @ ACCULINNA-2 was characterized in this work, in terms of amplitude and time resolution, neutron/gamma separation performance and detection efficiency in the detector,
- I also engage in the preparation and conduct of experiments,
- My wishes are not only to analyze the data but also to **master the physical foundations** of the models underlying the nuclear reactions description, then a path way for PhD @ JINR, excel at Nuclear Physics - a **real physicist**.

Much appreciated for your attention.!